



WORLD HEADQUARTERS
ONE KNOLLCREST DR.
P.O. BOX 371805
CINCINNATI, OHIO
45222-1805
513-761-9255
513-761-0467 FAX
1-800-999-0400

DEC 03 2001

K 012268

510(k) Summary

This summary of 510(k) safety and effectiveness is being supplied in accordance with the Safe Medical Device Act of 1990 and 21 C.F.R.

807.92(a)

1. Standard Textile Co., Inc. Contact Person: Brad Bushman
One Knollcrest Drive (513) 761-9255 Ext. 455
Cincinnati, Ohio 45237 Summary Prepared on 6/29/01

2. Device Name: TriMax Surgical Gown, non-sterile (75X reusable)
Common/Usual Name: Surgical Gown
Classification Name: Surgical Apparel 21 C.F.R. § 878.4040

3. Predicate Device: ComPel XTR® Surgical Gowns #K922753

4. All fabric components used in TriMax Surgical Gowns are made from 100% polyester.

TriMax Surgical Gown will function as surgical gowns when processed according to instructions through 75 complete wash, dry and sterilization cycles. These products will be manufactured and distributed as non-sterile surgical gowns that are intended to be sterilized and processed by health care facilities and/or contract sterilization/laundry companies

5. TriMax Surgical Gown are intended to be worn by operating room personnel during surgical procedures to protect both the surgical patients and the operating room personnel from transfer of microorganisms, body fluids, and particulate material.

There are no critical differences in the use of this product from currently marketed ComPel XTR® Surgical Gowns except for higher liquid resistance claims, additional viral resistance claims and sleeve seam performance claims. TriMax Surgical Gown have demonstrated that they will perform as intended when used as labeled.

6. The tests that have been successfully completed include:

- a. Flammability 16 CFR Part 1610.
- b. Barrier Performance
 - i. Viral Resistance ASTM #1671-97b
 - ii. Suter Hydrostatic Testing AATCC #127-1989
 - iii. Mullens Hydrostatic Testing ASTM D751-95 Procedure A
- c. Strength ASTM #D-1682-87
- d. Lint EDANA 220.0-96
- e. Toxicity - Cytotoxicity MEM Elution (MG023)
Acute Systemic Toxicity (ISO 10993)
- f. Primary Skin Irritation (ISO 10993)
- g. Sterilization - Product sold non-sterile; can be sterilized using prevacuum steam cycles.
- h. Durability through 75 processing (wash, dry and sterilization).
- i. Colorfastness to Commercial Laundering - AATCC #61-1993(4A).

To the best of my knowledge, all data and information in the 510(k) are truthful and accurate, and that no material fact has been omitted.

Bradley J. Bushman



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

Mr. Bradley J. Bushman
Director, Technical Resources
Standard Textile Company, Incorporated
One Knollcrest Drive
P.O. Box 371805
Cincinnati, Ohio 45237-1600

DEC 03 2001

Re: K012268
Trade/Device Name: Trimax
Regulation Number: 878.4040
Regulation Name: Surgical Gown
Regulatory Class: II
Product Code: FYA
Dated: October 15, 2001
Received: October 19, 2001

Dear Mr. Bushman:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.


Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements

of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

This letter will allow you to begin marketing your device as described in your Section 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 21 CFR Part 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4618. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its Internet address <http://www.fda.gov/cdrh/dsma/dsmamain.html>

Sincerely yours,

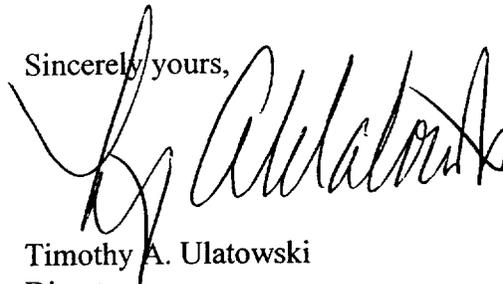

Timothy A. Ulatowski
Director
Division of Dental, Infection Control
and General Hospital Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

510(k) NUMBER: To be issued K012268

DEVICE NAME: TriMax Surgical Gown

INDICATIONS FOR USE:

TriMax Surgical Gown are intended to be worn by operating room personnel during surgical procedures to protect both the surgical patients and the operating room personnel from transfer of microorganisms, body fluids, and particulate material.

TriMax Surgical Gown will function as surgical gowns when processed according to instructions. The TriMax Surgical Gown are reusable through 75 wash, dry and sterilization cycles. They are manufactured and distributed as non-sterile surgical gowns that are intended to be sterilized and processed by health care facilities and/or contract sterilization/laundry companies.



(Division Sign-Off)
Division of Dental, Infection Control,
and General Hospital Devices

510(k) Number K012268

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE IF NEEDED.)

Concurrence of CDRH, Office of Device Evaluation (ODE)

Prescription Use _____
(Per 21 CFR 801.109)

OR

Over-The-Counter-Use
(Optional Format 1)