

AUG 31 1998

K982347



510(k) SUMMARY

NAME OF FIRM: DePuy ACE Medical Company
2260 East El Segundo Boulevard
El Segundo, CA 90245

510(k) CONTACT PERSON: Kathleen Dragovich
Regulatory Affairs Specialist
DePuy ACE Medical Company

TRADE NAME: DePuy ACE TiMAX™ Pilon Plate

COMMON NAME: Bone Fixation Plate

CLASSIFICATION: 888.3030 Single/multiple component metallic bone fixation appliances and accessories.

DEVICE CODE: 87HRS

SUBSTANTIALLY EQUIVALENT DEVICE: Synthes Cloverleaf Plate
Stainless Steel (241.83) & Titanium (441.83)

INTENDED USE:

- Pilon fractures - distal tibial intra-articular fractures
- High medial malleolar fractures
- Low Boot top type rotational distal extra-articular shaft fractures

DEVICE DESCRIPTION AND SUBSTANTIAL EQUIVALENCE RATIONALES:

The DePuy ACE TiMAX™ Pilon Plate is a fracture fixation plate intended for use in pilon fractures (distal tibial intra-articular fractures), high medial malleolar fractures, and low boot type rotational distal extra-articular tibial shaft fractures. The plate profile consists of a shaft portion with compression slots, a diamond-shaped structure with four screw holes and two k-wire guide holes for the distal metaphyseal region, and finally, an arm which wraps anteriorly to address the anterior crush fracture and facilitate articular surface reconstruction. The plate thickness is 1.6 mm in the shaft region and is decreased to 1 mm in the distal region to facilitate contouring and maintaining anatomic reduction of the fracture. The shaft portion is thicker for strength

The plate is supplied pre-formed to a contour, which closely matches the distal tibia anatomy. The general contour includes a medial bend from the shaft to the distal metaphyseal region combined with an internal rotation. The most distal profile includes the anterior arm with a large bend from the medial to the anterior surface with the bend apex located adjacent to the anterior strut.

The open architecture of the distal region allows easy contouring by the surgeon to accommodate the anatomical topography of the distal tibia and also to promote fracture healing. The screw holes have been designed to allow low profile interaction with the heads of the following screws: 3.5mm cortical screw, 4.0mm cancellous screw, and the periarticular screw. The plate will be offered in a right and left model with various lengths of the shaft region.

The DePuy ACE TiMAX™ Pilon Plate is manufactured from Titanium 6Al-4V ELI (per ASTM standard F136).

DePuy ACE TiMAX™ Pilon Plate was compared to the Synthes stainless steel cloverleaf plate and was found to have a higher yield bending strength and was lower bending stiffness.

Based on the above information, DePuy ACE Medical Company firmly believes that the new DePuy ACE TiMAX™ Pilon Plate is substantially equivalent to the Synthes Stainless Steel Cloverleaf Plate (pre-amendment device).



Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

AUG 31 1998

Mr. Paul Doner
Director, Regulatory and Clinical Affairs
DePuy ACE Medical Company
2260 East El Segundo Boulevard
El Segundo, California 90245-4694

Re: K982347
Trade Name: DePuy ACE TiMAX™ Pilon Plate
Regulatory Class: II
Product Code: HRS
Dated: July 2, 1998
Received: July 6, 1998

Dear Mr. Doner:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.


If your device is classified (see above) into either class II (Special Controls) or class III (Pre-market Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the current Good Manufacturing Practice requirement, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic (QS) inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

Page 2 - Mr. Paul Doner

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4659. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its internet address "<http://www.fda.gov/cdrh/dsmamain.html>".

Sincerely yours,

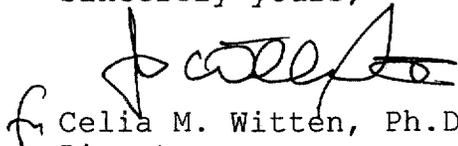

Celia M. Witten, Ph.D., M.D.
Director
Division of General and
Restorative Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

510(k) Number (if known) K982347

Device Name: **DePuy ACE TiMAX™ Pilon Plate**

Indications for Use:


- Pilon fractures - distal tibial intra-articular fractures
- High medial malleolar fractures
- Low Boot top type rotational distal extra-articular shaft fractures

Concurrence of CDRH, Office of Device Evaluation

Prescription Use X
(Per 21 CFR 801.109)

OR

Over-The-Counter _____

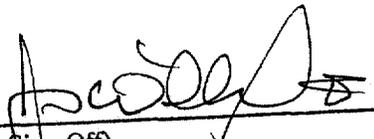

(Division Sign-Off)
Division of General Restorative Devices
510(k) Number K982347