

DEC 17 1998

K984325



**Bio-Rad  
Laboratories**

Diagnostics Group  
9500 Jeronimo Road  
Irvine, California 92618-2017  
Telephone: (949) 598-1200

---

## 510(k) Summary

### Submitter

Bio-Rad Laboratories  
9500 Jeronimo Road  
Irvine, CA  
(949)598-1285  
Fax (949)598-1555

### Contact Person

Elizabeth Platt

### Date of Summary Preparation

December 02, 1998

### Device (Trade & Common Name)

Architect Ferritin MasterCheck

### Classification Name

Class I, 75JJX  
CFR 862.1660: Single (Specified) Analyte Controls (Assayed and Unassayed)

### Devices to Which Substantial Equivalence is Claimed

Document Serum Multi-Analyte Verification Test Set  
Casco Standards  
Yarmouth, ME  
K950469

### Statement of Intended Use

Architect Ferritin MasterCheck is intended for use in the verification of sensitivity, calibration linearity, and reportable range of the Ferritin assay on the Abbott Architect i System.

Description of the Device

Architect Ferritin MasterCheck Level 0 contains HEPES buffer with protein (bovine) stabilizers.

Architect Ferritin MasterCheck Levels 1, 2, 3 and 4 contain ferritin (human) prepared in HEPES buffer with protein (bovine) stabilizers.

Preservative: Antimicrobial Agent.

Statement of How Technological Characteristics Compare to Substantial Equivalence Device

A table is provided below comparing the similarities between the Bio-Rad Architect Ferritin MasterCheck and the devices to which substantial equivalence is claimed.

	Architect Ferritin MasterCheck	Casco Standards Document Serum Multi-Analyte Verification Test Set
Intended Use	Verification of sensitivity, calibration linearity, and reportable range of the Ferritin assay on the Abbott Architect <i>i</i> System.	<i>In vitro</i> diagnostic use in the quantitative determination of linearity, calibration verification and verification of reportable range using automated, semi-automated and manual methods.
Form	Liquid	Liquid
Matrix	HEPES buffer with protein (bovine) stabilizers	Human Serum
Storage	2-8°C	-10 to -20°C
Analytes	Ferritin	Multiple
Open Vial Claim	3 Days at 2-8°C.	30 Days at 2-8°C.
Differences	Calibration verifier for the Architect Ferritin assay	Calibration verifier for multiple analytes.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

DEC 17 1998

Ms. Elizabeth Platt  
Regulatory Affairs Supervisor  
Bio-Rad Laboratories  
Diagnostics Group  
9500 Jeronimo Road  
Irvine, California 92618-2017

Food and Drug Administration  
2098 Gaither Road  
Rockville MD 20850

Re: K984325  
Trade Name: Architect Ferritin MasterCheck  
Regulatory Class: I  
Product Code: JJY  
Dated: December 2, 1998  
Received: December 3, 1998

Dear Ms. Platt:


We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

If your device is classified (see above) into either class II (Special Controls) or class III (Premarket Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the Current Good Manufacturing Practice requirements, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic QS inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4588. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance, at its toll-free number (800) 638-2041 or (301) 443-6597, or at its internet address "<http://www.fda.gov/cdrh/dsma/dsmamain.html>".

Sincerely yours,



Steven I. Gutman, M.D., M.B.A.  
Director  
Division of Clinical  
Laboratory Devices  
Office of Device Evaluation  
Center for Devices and  
Radiological Health

Enclosure

510(k) Number: K984325

Device Name: Architect Ferritin MasterCheck


Indications for Use:

Architect Ferritin MasterCheck is intended for use in the verification of sensitivity, calibration linearity, and reportable range of the Ferritin assay on the Abbott Architect *i* System.

(PLEASE DO NOT WRITE BELOW THE LINE-CONTINUE ON ANOTHER PAGE IF NEEDED)

---

(Concurrence of CDRH, Office of Device Evaluation)

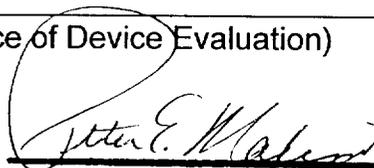  
**(Division Sign-Off)**  
**Division of Clinical Laboratory Devices**  
**510(k) Number** K984325

Prescription Use

OR Over-The Counter Use