

Caution: Federal law restricts this device to sale by or on the order of a physician.

1. INTENDED USE

ETI-EBK PLUS is an *in vitro* enzyme immunoassay (EIA) intended for use in the qualitative detection of hepatitis Be antigen (HBeAg) in human serum or plasma (EDTA, citrate or heparin). The ETI-EBK PLUS is intended for manual use and with the Biochem Immunosystems Labotech/ETI-Lab automated instrument.

The detection of HBeAg is indicative of a laboratory diagnosis for active HBV replication, usually correlating with viremia. A reactive test is presumptive laboratory evidence for infection with hepatitis B virus (HBV). Further HBV serological marker testing is required to define the specific disease state. The ETI-EBK PLUS assay's performance has not been established for the monitoring of HBV disease or therapy.

Assay performance characteristics have not been established when the DiaSorin ETI-EBK PLUS HBeAg assay is used in conjunction with other manufactures' assays for specific HBV serological markers. Users are responsible for establishing their own performance characteristics.

The performance characteristics of this assay have not been established for newborn testing.

Caution: Performance characteristics for the DiaSorin ETI-EBK PLUS were largely determined using archival specimens which may not be representative of test results obtained from fresh specimens. Laboratories are advised that they should monitor patient results using other appropriate HBV serological markers or retest questionable specimens with another legally-marketed HBeAg assay.

2. SUMMARY AND EXPLANATION OF THE TEST

Hepatitis is an inflammatory disease of the liver that can severely damage the organ. The disease can result from non-infectious causes—such as biliary obstruction, biliary cirrhosis, Wilson's disease, drug toxicity, and drug hypersensitivity reactions—or from infectious viral and bacterial agents (1). Viral hepatitis is commonly caused by one of several viruses: hepatitis A virus (HAV), hepatitis B virus (HBV), hepatitis C virus (HCV), hepatitis D (delta) virus (HDV) in conjunction with HBV (1, 2), hepatitis E virus (HEV), and other as yet uncharacterized or partially characterized hepatitis viruses (non-A-E). Other viruses, including yellow fever virus, human cytomegalovirus, Epstein-Barr virus, rubella virus, herpes simplex virus, varicella-zoster virus, and some enteroviruses, can cause forms of hepatitis (1, 2).

Hepatitis B, also known as serum hepatitis, is endemic throughout the world (3-5). The infection is spread primarily through percutaneous contact with infected blood, e.g., sharing of needles by drug addicts or transfusion of blood products that have not been screened for HBV (1, 3, 6, 7). The virus is also found in virtually every type of human body fluid and has been known to be spread through oral and genital contact (1, 3, 6, 7). HBV can be transmitted from mother to child during delivery through contact with blood and vaginal secretions; it is not commonly transmitted transplacentally (6).

The incubation period for hepatitis B averages 90 days (range 40-180 days). Common symptoms include malaise, fever, gastroenteritis, and jaundice (icterus) (8). HBV infection can lead to

a) icteric hepatitis, b) subclinical anicteric hepatitis, c) fulminant hepatitis, or d) chronic active or persistent hepatitis (1, 3). Over 90% of adult patients with hepatitis B completely recover from acute illness, approximately 1% die of fulminant hepatitis, and approximately 3 to 5% become chronic or persistent carriers (1-3).

The complete hepatitis B virus, also called the Dane particle, is composed of an outer surface or envelope that carries the hepatitis B surface antigen (HBsAg) (9, 10). The envelope surrounds an inner core that contains the hepatitis B core antigen (HBcAg) (11-13). Inside the core is the HBV deoxyribonucleic acid (DNA) genome. Another antigen, the hepatitis B e antigen (HBeAg), is a viral core protein found in the bloodstream during active replication of HBV (1, 14).

Because HBV is very difficult to isolate in cell culture, hepatitis B diagnosis has been based on detection of serologic markers. Early methods used to detect serologic markers were immunodiffusion and counterimmunoelectrophoresis (3). Methods commonly used now include hemagglutination, immune adherence, latex agglutination, radioimmunoassay (RIA), and enzyme immunoassay (ELISA) (1, 3). The ELISA and RIA methods are the most widely utilized because of their high analytical sensitivity, analytical specificity, and ease of use.

When determining the stage of disease caused by HBV the HBV serologic markers commonly tested for are HBsAg, antibody to HBsAg (anti-HBs), total antibody to HBcAg (total anti-HBc), immunoglobulin M antibody to HBcAg (IgM anti-HBc), HBeAg, and antibody to HBeAg (anti-HBe). Testing for these markers helps to determine the presence of past or ongoing HBV infection, the acute or chronic stage of the disease, response to therapy, and/or the immune status of the patient (1, 15).

In the normal course of acute hepatitis B infection, HBeAg, along with HBsAg and HBV-DNA, become detectable in a patient's serum during the incubation period, before the onset of clinical symptoms (2). With the appearance of clinical symptoms, levels of HBeAg, HBsAg and HBV-DNA peak and then begin to decline (2, 15, 16). HBeAg usually disappears prior to the disappearance of HBsAg; however, in a minority of cases the opposite situation occurs. Anti-HBe appears in the serum after HBsAg is no longer detectable. Anti-HBe may be detectable in serum for several years after the patient's recovery from acute HBV infection (2).

Diagnostically, the presence of HBeAg in serum indicates active replication of HBV (17); this may occur in a person with acute hepatitis B or in a person who has become a chronic HBV carrier, with persistence of HBsAg. Chronic persistence of HBeAg is often associated with chronically elevated liver enzymes. Persons with HBeAg-positive results are considered highly infectious for hepatitis B (18); however, the absence of HBeAg does not denote absence of infectivity.

A mutant strain of HBV has been recently observed (19) in patients from Asia or the Mediterranean basin. This strain is characterized by a mutation in the precore region of the viral genome which prevents HBeAg secretion despite ongoing viral replication and high HBV-DNA levels. This uncommon strain causes a situation where HBeAg is serologically undetectable despite ongoing viral replication and active liver disease.

3. PRINCIPLE OF THE PROCEDURE

ETI-EBK PLUS uses monoclonal antibodies to hepatitis Be antigen as the basis for this enzyme immunoassay. The assay is a direct, non-competitive test based on the use of polystyrene microwells coated with mouse monoclonal antibodies to HBeAg. An enzyme tracer containing horseradish peroxidase-labeled mouse monoclonal antibodies to HBeAg detects any captured HBeAg from the patient's specimen. The monoclonal antibodies are of the IgG1-k class and are directed to the secreted form of HBeAg.

In the assay procedure, patient specimens and controls are incubated with incubation buffer in antibody-coated microwells. If HBeAg is present in a specimen or control, it binds to the antibody.

Excess sample is removed by a wash step, and the enzyme tracer is then added to the microwells and allowed to incubate. The enzyme tracer binds to any antigen-antibody complexes present in the microwells. Excess enzyme tracer is removed by a wash step, and a chromogen/substrate solution is added to the microwells and allowed to incubate. If a sample contains HBeAg, the bound enzyme (horseradish peroxidase) chemically reduces the substrate peroxide, which concurrently oxidizes the chromogen tetramethylbenzidine (TMB) to a blue color (650 nm). The blue color turns to yellow (450 nm) after addition of the stop solution. If a sample does not contain HBeAg, the microwell will be colorless after the chromogen/substrate solution is added and will remain colorless after the stop solution is added. Color intensity, which is measured spectrophotometrically, is indicative of the concentration of HBeAg. Absorbance value readings for patient specimens are compared to a cutoff value determined from the mean of the calibrators.

4. REAGENTS AND OTHER MATERIALS PROVIDED

Catalog Number	Product Description	Quantity/ Volume
P001930	ETI-EBK PLUS	96 tests
	Coated Strips Microwells coated with mouse monoclonal antibodies to HBeAg (IgG1-k class, directed to the secreted form of HBeAg).	Twelve 8-well strips (contained in one pouch)
	Enzyme Tracer Horseradish peroxidase-labeled mouse monoclonal antibody to HBeAg, buffer, protein stabilizers (IgG1-k class, directed to the secreted form of HBeAg). Preservative: 0.2% ProClin 300.	0.5 mL
	Tracer Diluent Buffer, protein stabilizers. Preservative: 0.2% ProClin 300.	14.7 mL
	Calibrator (Human) Human serum/plasma non-reactive for all known HBV markers. Preservative: 0.2% ProClin 300.	3.3 mL
	Negative Control (Human) Human serum/plasma non-reactive for all known HBV markers. Preservative: 0.2% ProClin 300.	3.3 mL
	Positive Control HBeAg (recombinant DNA), protein stabilizers. Preservative: 0.2% ProClin 300.	2.5 mL
	Incubation Buffer Buffer, protein stabilizers, an inert blue dye. Preservative: 0.2% ProClin 300.	8 mL
	Wash Buffer (concentrate)* Buffer, detergents, preservatives.	40 mL
	Chromogen/Substrate* Tetramethylbenzidine/hydrogen peroxide system at pH 5.3.	16 mL
	Stop Solution* 1N sulfuric acid. Caution: corrosive.	30 mL
	Strip Sealers	24
	Plate Sealers	2
	Pouch Sealer	1

** All lots of wash buffer concentrate, chromogen/substrate and stop solution are interchangeable between assay kits.*

5. WARNINGS AND PRECAUTIONS

- For *in vitro* diagnostic use only.
- The human blood source material used to prepare this product (e.g. Calibrator and Negative Control) has been tested and found non-reactive for HBsAg, antibodies to HCV, and antibodies to HIV-1 and HIV-2 by FDA approved methods. Because no test method can offer complete assurance that laboratory specimens do not contain HIV, hepatitis B virus, or other infectious agents, specimens should be handled at the BSL 2 as recommended for any potentially infectious human serum or blood specimen in the CDC-NIH manual, Biosafety in Microbiological and Biomedical Laboratories, 4th Edition, May 1999 and NCCLS Approved Guideline M29-A, Protection of Laboratory Workers from Instrument Biohazards and Infectious Disease Transmitted by Blood, Body Fluids, and Tissue. (20, 21, 22).
- All specimens, reagents, and controls should be handled as if capable of transmitting disease. Follow standard precautions for handling infectious agents during all procedures:
 - Do not pipette by mouth.
 - Do not eat, drink, smoke, or apply cosmetics in areas where specimens are handled.
 - Wear protective clothing such as lab coats, protective glasses, and disposable gloves when handling specimens and assay reagents. Wash hands thoroughly afterwards.
 - Perform all work with infectious materials in a designated area.
- Dispose of all specimens and used assay materials as if capable of transmitting disease:
 - Decontaminate liquid wastes, including those containing neutralized acid, either:
 - (a) by autoclaving for 60 minutes at 121°C; or
 - (b) by treating with a 1:10 or 1:100 dilution of household bleach (sodium hypochlorite concentration approximately 5%). The wastes should remain in contact with the sodium hypochlorite solution for 30 minutes for effective decontamination, after which they can be disposed of in the sink (20, 22). Do not autoclave solutions containing sodium hypochlorite.
 - Autoclave non-ignitable solids for 60 minutes at 121°C.
 - Incinerate disposable ignitable materials.
- Performing the assay outside the time and temperature ranges provided may produce invalid results. Assays not falling within the established time and temperature ranges must be repeated.
- Use only dispersing equipment that has been calibrated to deliver accurate volumes, per the laboratory's standard procedures.
- **WARNING: Chromogen/substrate and the stop solution contain ingredients that can irritate skin and cause eye damage. Handle them with care. Avoid getting them in eyes or on skin or clothing. In case of contact with skin or eyes, immediately flush the affected area with water for 15 minutes. For eyes, obtain medical attention.**

Reagents containing ProClin 300 may cause allergic reactions. Avoid prolonged contact with skin. Wash thoroughly after handling.

6. REAGENT PREPARATION

- Bring reagents to room temperature (20-25°C).
- The coated strips, calibrator, negative and positive controls, incubation buffer, chromogen/substrate and stop solution are provided ready to use.
Note - Use clean, plastic containers or acid-washed glassware for preparing the following solutions. A clean, dedicated dispenser is recommended for the working enzyme tracer to avoid contamination.
- **Working enzyme tracer.** Bring reagents to room temperature (20-25°C). To prepare the working enzyme tracer, dilute the enzyme tracer 1:50 with tracer diluent (see chart below). After dilution, the working enzyme tracer can be used for one week if stored at 2-8°C.
Caution - Verify that the total volume prepared is sufficient for the number of tests included in the run. Use a clean container for each dilution and label the container with the reagent name, lot number of kit, lot number of reagent, plus the date of preparation and date of expiration of the working enzyme tracer.

Number of Strips	Enzyme Tracer (µL)	Tracer Diluent (µL)	Total Volume (mL)
2	48	2352	2.4
4	80	3920	4.0
6	112	5488	5.6
8	144	7056	7.2
10	176	8624	8.8
12	208	10192	10.4

Note - Sufficient reagents are provided to allow for six runs per kit.

- **Wash solution.** To prepare the working wash buffer, dilute the wash buffer concentrate (40 mL) to 1000 mL (1.0 L) with distilled or deionized water. If crystallization has occurred at 2-8°C, warm the wash buffer concentrate to 37°C and mix well before diluting. Water used for wash buffer dilution should be stored in a clean, non-metallic container to prevent contamination with peroxidase-inactivating substances. Record on the storage vial the expiration date and date of preparation of the working wash buffer. The working wash buffer can be stored for one week at 2-8°C.
Smaller volume users may prepare less than 1 L of working wash buffer at a time if desired. If diluting only a portion of the wash buffer concentrate, check concentrate for crystallization. If crystallization has occurred during storage, warm the wash buffer concentrate to 37°C and mix well to eliminate crystals before removing aliquot for dilution.
Note - All lots of wash buffer concentrate are interchangeable.
- Working wash buffer containers should be thoroughly cleaned with 70% ethanol and thoroughly rinsed with distilled or deionized water before preparation of the next batch of working wash buffer.

7. REAGENT STORAGE AND HANDLING INSTRUCTIONS

- Store the test components in the refrigerator at 2-8°C away from intense light. Allow them to reach room temperature (20-25°C) before use. Return the test components to the refrigerator after use.
- Do not expose the test components to intense light, direct sunlight, or temperatures above 25°C. Do not freeze the kit.

- When stored as directed, test components will remain stable until expiration dates printed on their labels.
- Keep unused coated strips sealed in their pouches until time for use. Allow the pouch to reach room temperature (20-25°C) before opening it. Return any unused strips to the pouch as soon as possible; seal the pouch with the pouch sealer and refrigerate pouch at 2-8°C.
- After dilution, the working enzyme tracer can be stored for one week at 2-8°C.
- After dilution, the working wash buffer can be stored for one week at 2-8°C.

8. REAGENT INSTABILITY OR DETERIORATION

- The chromogen/substrate may have a slightly blue tinge. If the chromogen/substrate turns a darker blue, it may have become contaminated and should be discarded.
- Any reagent that contains visible particulate matter should be discarded.

9. SPECIMEN COLLECTION AND PREPARATION

- **This assay is not designed to test body fluids other than human serum or plasma.**
- Specimens containing precipitate may give inconsistent test results. Do not test specimens containing particulate material, or grossly hemolyzed or lipemic specimens.
- There is a specimen dilutional effect with citrated plasma due to the liquid nature of this anticoagulant. Borderline or high-negative results obtained from citrated specimens should be retested using serum as the matrix.
- Each assay requires 100 µL human serum or plasma. EDTA, citrate or heparin anticoagulants have been tested and may be used with this assay. Follow manufacturer's instructions carefully when using plasma collection containers with anticoagulants.
- Do not test heat inactivated samples with this assay.
- Samples that are to be used fresh may be stored for up to 2 hours at 2-8°C in the presence of clots. Serum separated from the clot may be stored at 2-8°C up to 48 hours, but then must be frozen and stored deep-frozen (at -20°C or below) in sterile containers until use (23). If sample is stored frozen, mix thawed sample well before testing. It has been shown that up to three freeze-thaw cycles do not interfere with the assay.
- For shipping, specimens should be frozen at -20°C or below and shipped with dry ice. Temperature level during entire shipment should be no greater (warmer) than -20 °C. Pack specimens in compliance with government regulations covering the transportation of etiologic agents (24).

10. MANUAL ASSAY PROCEDURE

Materials Provided

ETI-EBK PLUS

Coated Strips
 Enzyme Tracer
 Tracer Diluent
 Calibrator (Human)
 Negative Control (Human)
 Positive Control

Wash Buffer (Concentrate)
 Chromogen/Substrate
 Stop Solution
 Strip Sealers
 Plate Sealers
 Pouch Sealer.

Incubation Buffer

Materials Required But Not Provided

Microwell plate washer - The following instrument specifications are recommended for the kit performance:

Volume dispensed: 350-370 μL

Number of wash cycles: 5

Soak time: 30 seconds

Aspirate the last aliquot of dispensed liquid: yes.

Note - The volume of each microwell is approximately 400 μL . Make sure the volume of working wash buffer dispensed into each well does not cause the wells to overflow. If the wells overflow, set the washer to dispense less working wash buffer.

Microwell plate reader - The following instrument specifications are recommended for the kit performance:

Wavelength: dual wavelength, 450 nm and 600-650 nm

Bandwidth: ≤ 10 nm

Absorbance range: 0 absorbance units to ≥ 3 absorbance units

Repeatability: better than or equal to 0.005 absorbance units, or 1%, whichever is greater

Linearity or accuracy: better than or equal to 0.010 absorbance units, or 2%, whichever is greater

Drift: less than 0.005 absorbance units per hour.

Incubator, $37^\circ\text{C} \pm 1^\circ\text{C}$.

Note - Gravity convection incubators are recommended. Forced-air incubators may cause edge effects. Do not use water baths as incubators.

Micropipettes with disposable clean tips (50 μL and 100 μL).

Note - Suggested specifications for micropipettors (based on gravimetric testing) are:

50 μL : accuracy $\pm 3\%$, precision 2%

100 μL : accuracy $\pm 2\%$, precision 1%.

Miscellaneous clean glass or plastic containers

Hazardous waste disposal materials

Disposable gloves

Distilled or deionized water

Pipetter-diluter (optional)

Multichannel pipetter (optional)

Pipette tips for multichannel pipetter (if multichannel pipetter is used)

Disposable reagent reservoirs (if multichannel pipetter is used)

Printer compatible with microwell reader.

Automated Procedure Using Biochem Immunosystems Labotech/ETI-Lab Instrument.

See the Labotech (ETI-LAB) instrument Instruction Manual.

Assay Procedure

Perform all assay steps in the order given and without any delays between the steps. A cutoff value is calculated for each plate based on the absorbance values of the calibrators run on that plate. A maximum of one plate should be set up (completed through the first incubation step) at a time. If multiple plates are being run as a batch, each plate must be treated as a single entity; i.e., the calibrators, controls and patient specimens for the plate must be added and the incubation time started before moving on to the next plate. Proper instrument maintenance is critical for good

assay performance. Follow the manufacturer's instructions for performing instrument warm-up, quality control, calibration and maintenance procedures on all equipment used in this assay.

Note: All steps must be completed within four hours. Calibrator, positive and negative controls must be run with each plate of patient specimens.

1. Prepare assay reagents. Allow all test components to reach room temperature (20-25°C). Prepare working wash buffer and working enzyme tracer according to the directions given in Section 6, Reagent Preparation. Refer to the chart in Section 6 to ensure preparation of sufficient reagent volumes for the number of tests included in the run.

2. Prepare coated plate. Prepare enough microwells for the calibrators, controls and samples to be tested. Allow one blank well containing only chromogen/substrate and stop solution in well A1. Allow one well for each patient sample. The calibrator must be tested in triplicate and the negative and positive controls tested in singlet. Calibrators are to be placed in wells B1, C1 and D1; negative control is to be placed in well E1; positive control is to be placed in well F1 (for details, refer to the recommended plate map at the end of this section). Test calibrator and controls as you would patient specimens.

Coated strips may be separated. Avoid handling the bottoms of the microwells because scratches or marks could affect the reading of test results. Store unused strips in their original pouch, seal the pouch carefully, and refrigerate at 2-8°C.

3. Add incubation buffer. Add 50 µL incubation buffer to all microwells (except for the blank well).

4. Add samples and controls. If sample was stored frozen, mix thawed sample well (vortex) before proceeding. Add 100 µL of each calibrator, control or sample to its respective microwell. To avoid cross-contamination, use a clean micropipette tip to dispense each calibrator, control or specimen. Record the microwell position of each calibrator, control or patient specimen on a laboratory data sheet.

Incubation buffer is light blue in color. On addition of calibrators, controls or samples, the color will turn to green or dark blue. This color change may vary from sample to sample, but it will always be visible.

5. Incubate. Cover the microwells with a plate or the strip sealer provided with this kit. Use a roller to affix the sealer or press firmly by hand around microwell and plate edges to ensure that the sealer is firmly attached over the entire strip or plate. Tap the coated plate gently to release any air bubbles trapped in the liquid making sure samples do not splash onto the sealer. Ensure that all microwells are filled equally. Incubate the microwells for **2 hours ± 10 minutes at 37°C ± 1°C.**

6. Wash coated plate. Remove and discard the sealer. Aspirate the liquid from the microwells and wash each well five times as follows: Deliver 350-370 µL of working wash buffer to each microwell, let the wells soak for 30 seconds, and then aspirate the working wash buffer completely from each microwell. Microwell plate washers vary by manufacturer. Make sure the volume of working wash buffer dispensed into each well completely fills the well but does not cause the well to overflow.

7. Remove excess working wash buffer. Ensure that all microwells are aspirated completely before proceeding. With some washers it may be necessary to invert the microplate and tap it forcefully on a paper towel to effectively remove residual working wash buffer.

8. Add working enzyme tracer. Immediately add 100 µL working enzyme tracer to each well (except for the blank well).

9. Incubate. Cover the microwells with a plate or strip sealer using the sealers provided for this kit. Ensure that sealer is applied correctly (see Step 5). Tap the coated plate gently to release any air bubbles trapped in the liquid. Ensure that all microwells are filled equally. Incubate the microwells for 60 ± 5 minutes at $37^\circ\text{C} \pm 1^\circ\text{C}$.

Warning - Timing of this incubation step is critical.

10. Wash coated plate. Remove and discard the sealer. Aspirate the working enzyme tracer from the microwells and wash them as described in Steps 6 and 7.

11. Add chromogen/substrate. Immediately add 100 μL chromogen/substrate to all microwells, including the blank well.

Note - The chromogen/substrate may have a slightly blue tinge. However, if it turns a darker blue, it may have become contaminated and should be discarded.

12. Incubate. Incubate the microwells for 30 ± 2 minutes at room temperature ($20\text{-}25^\circ\text{C}$). Avoid exposing the microwells to direct or intense light. Do not exceed the time limits of this incubation.

13. Add stop solution. Add 100 μL stop solution to each microwell in the same order as chromogen/substrate was added.

14. Read results. Within one hour after addition of stop solution, read the absorbance values of the calibrators, negative control, positive control, and samples with the microwell reader set at 450/630 nm in the bichromatic mode. If time before reading exceeds one hour the tests must be discarded and specimens retested. Check for and remove air bubbles before reading results. Record the absorbance value for each calibrator, control and sample.

Note - Blank the instrument on the blank well. The absorbance of the blank well containing only chromogen/substrate and stop solution (see Step 2 in Section 10, Procedure) is evaluated as described in the QC section. The value for the blank well should be recorded and subtracted from each calibrator, control and sample value before calculating mean values and cutoff, and before interpreting results.

15. Perform assay quality control procedures. Before evaluating results, perform quality control procedures (see Section 11, Quality Control).

16. Perform equipment quality control and maintenance procedures. Proper instrument maintenance including calibration is critical for good assay performance. Follow the manufacturer's instructions for performing quality control and maintenance procedures on all equipment used in this assay.

Recommended Plate Map

	1	2	3	4	5	6	7	8	9	10	11	12
A	BLK	S3										
B	CAL1	S4										
C	CAL2	S5										
D	CAL3	S6										
E	NC	S7										
F	PC	S8										
G	S1	etc.										S89

H	S2										S90
---	----	--	--	--	--	--	--	--	--	--	-----

11. QUALITY CONTROL

The Negative and Positive Controls are intended to monitor for substantial reagent failure. The Positive Control will not ensure precision at the assay cutoff.

The quality control material furnished is in a serum matrix. It may not adequately control the assay for plasma specimens. The user should provide alternate control material for testing of plasma matrices.

Additional controls may be tested according to guidelines or requirements of local, state, and/or federal regulations or accrediting organizations.

Use the following steps to validate quality control. References 25 and 26 provide guidance on quality control recommendations. Record the results on the QC Verification Worksheet provided for the assay.

Compute the mean absorbance value for the calibrator.

Always evaluate mean calibrator value and negative and positive control values for each plate when running more than one plate in a batch. Be sure to compare the absorbance value of each patient sample with the cutoff value computed for the plate containing that sample.

1. Evaluate the absorbance value of the substrate blank.

Blank the instrument on the blank well containing only chromogen/substrate and stop solution (see Step 14 in Section 10, Procedure). The absorbance value for the blank well must be between 0.000 and 0.150 for the assay to be valid. If the absorbance value of the substrate blank is less than 0.000 or greater than 0.150, the run must be repeated.

Note - Subtract the substrate blank absorbance value from each absorbance value before performing the following evaluations.

2. Evaluate the mean calibrator absorbance value (Cal \bar{x}).

Each calibrator absorbance value (after subtraction of the blank) must be greater than -0.020 and less than 0.120 .

$$-0.020 < \text{Cal} < 0.120$$

If one of the calibrator absorbance values does not meet this criterion, it should be discarded and the mean value recalculated using the remaining two values. If more than one calibrator absorbance values do not meet this criterion, the run is invalid and must be repeated.

Example 1: Calculation of mean of calibrators

Calibrator Well	Absorbance	minus blank abs.	final calibrator abs.
B1	0.044	0.030	0.014
C1	0.040	0.030	0.010
D1	0.047	0.030	0.017

Total absorbance			0.041
------------------	--	--	-------

$$\text{Mean of calibrators (Cal } \bar{x}) = \frac{\text{Total absorbance}}{3} = \frac{0.041}{3} = 0.014.$$

The mean calibrator absorbance value must be greater than -0.020 and less than 0.120 .

$$-0.020 < \text{Cal } \bar{x} < 0.120$$

If the mean calibrator absorbance value does not meet this criterion, the run is invalid and must be repeated.

3. Evaluate the negative control absorbance value (NC).

After subtracting the substrate blank absorbance the negative control absorbance value must be greater than -0.020 and less than 0.120 .

$$-0.020 < \text{NC} < 0.120$$

If the negative control absorbance value does not meet this criterion, the run is invalid and must be repeated.

4. Evaluate the positive control absorbance value (PC).

After subtracting the substrate blank absorbance the positive control absorbance value must be greater than 0.500 and less than 2.500 .

$$0.500 < \text{PC} < 2.500$$

If the positive control absorbance value does not meet this criterion, the run is invalid and must be repeated.

5. Evaluate the difference between the positive control absorbance value and the negative control absorbance value.

The difference between the positive control absorbance value and the negative control absorbance value must be greater than 0.450 .

$$\text{PC} - \text{NC} > 0.450$$

If the difference between the positive control absorbance value and the negative control absorbance value does not meet this criterion, the run is invalid and must be repeated.

Example 2: Calculation of difference between PC and NC

Positive control absorbance (PC)	= 1.574
Negative control absorbance (NC)	= 0.014
Difference (PC - NC) = 1.574 - 0.014	= 1.560

12. QUALITY CONTROL PROBLEM SOLVING

It is important to follow the assay procedure precisely. If calibrator or control values are not within acceptable limits (see Section 11, Quality Control) or results differ markedly from those expected, check these assay variables:

- Check incubator, incubation times, and temperatures.

- A properly functioning washer is critical to the assay. Ensure that the washer is filling and aspirating all wells, that no probes are plugged, and that the probes are placed correctly in the microwells. No fluid should be left in the wells at the end of the wash step.
- Be sure that wells do not dry out between washing and addition of the next reagent. Add reagent within 2 minutes of removal of the plate from the washer. If a probe (or probes) on the washer becomes plugged during washing, identify the affected microwell(s) but continue with the assay procedure. Retest the affected specimen(s). To unplug probes, refer to the washer operator's manual.
- Check that all reagents and specimens are at room temperature (20-25°C) before starting the assay.
- Check that all reagents are within the expiration date, that appropriate assay kit components and ancillaries are used, and that there are no visible signs of contamination such as cloudiness or precipitates.
- Avoid cross-contamination of reagents and wells. If multichannel pipette tips have been contaminated, replace the tips.

13. INTERPRETATION OF RESULTS

The presence or absence of HBeAg is determined by comparing the absorbance values of patient samples with a cutoff value. The cutoff value is determined for each plate based on the absorbance values of the calibrators run on that plate. Be sure to compare the absorbance value of each patient sample with the cutoff value computed for the plate containing that sample.

Calculation of Cutoff Value

The cutoff value is determined by adding 0.060 to the mean absorbance of the calibrator values after subtraction of the substrate blank.

$$\text{CUTOFF} = \text{Cal } \bar{X} + 0.060$$

Example 3: Calculation of cutoff value

Calibrator mean absorbance	0.014
Constant	+ 0.060
Cutoff value for this run	0.074

The cutoff was established by testing 348 samples (174 volunteer blood donors and 172 hospitalized patients) with three lots of ETI-EBK PLUS. The results were examined as the difference (delta) between single sample absorbance and calibrator absorbance. In both populations, 99% had delta values less than 0.037.

Interpretation of Results

Absorbance Values	Result	Interpretation
Manual assay: absorbance < 90% x Cutoff Labotech/ETI-LAB assay: absorbance < 80% x Cutoff	Negative	HBeAg not detected by ETI-EBK PLUS. This result should not be used alone but in conjunction with other hepatitis B serological markers to determine disease state.
Manual assay: absorbance within 90-110% of Cutoff Labotech/ETI-LAB assay:	Equivocal	Presence of HBeAg indeterminate by ETI-EBK PLUS. Specimen should be retested using ETI-EBK PLUS kit to establish presence or

absorbance within 80-120% of Cutoff		absence of antigen. If a specimen is found repeatedly equivocal, the pattern of other hepatitis B serological markers should be used to identify status of disease, or another sample should be collected and tested at a later date.
Manual assay: absorbance > 110% x Cutoff Labotech/ETI-LAB assay: absorbance > 120% x Cutoff	Positive	HBeAg detected by ETI-EBK PLUS. This result should not be used alone but in conjunction with other hepatitis B serological markers to determine disease state.

Note - The magnitude of the measured result, above the cutoff, is not indicative of the total amount of antigen present.

Example 4: Interpretation of samples

Cutoff = 0.074

Equivocal Zone: Manual assay = 0.067 – 0.081; Automated Assay (on Labotech/ETI-Lab Instrument) = 0.059 – 0.089

Sample No. 1 absorbance = 0.041

Sample No. 2 absorbance = 1.186

Sample No. 1 should be considered negative for HBeAg; sample No. 2 should be considered positive for HBeAg.

14. LIMITATIONS OF THE PROCEDURE

- Results obtained from immunosuppressed patients should be interpreted with caution.
- This assay is not designed to test body fluids other than human serum or plasma.
- Any laboratory test result should be interpreted in conjunction with the patient's clinical presentation and the results of other diagnostic tests. A negative result on a given laboratory assay does not by itself rule out the possibility of infection.
- Very high concentrations of the monoclonal antibody used in the coated strips (approx. 83 times higher than used in the assay) have been shown to react with HBcAg.
- The prevalence of the analyte will affect the assay's predictive value.
- Assay performance characteristics have not been established when the DiaSorin ETI-EBK PLUS HBeAg assay is used in conjunction with the other manufacturers' assays for specific HBV serological markers. Users are responsible for establishing their own performance characteristics.
- Performance characteristics have not been established for any other automated instrument than the Biochem Immunosystems Labotech/ETI-Lab automated instrument. If another automated instrument is used the user is responsible for establishing their own assay performance characteristics.
- Specimens from patients receiving preparations of mouse monoclonal antibodies for therapy or diagnosis may contain human anti-mouse antibodies (HAMA). Such specimens may produce false positive result when tested with a two-site sandwich immunoassay such as the DiaSorin ETI-EBK PLUS assay. Specimens from these individuals should not be tested with this assay.
- The analytical sensitivity of the DiaSorin ETI-EBK PLUS assay has been determined to be approximately 0.2 PEI U/mL.

15. EXPECTED VALUES

The 236 prospective samples used in the expected values study for the DiaSorin ETI-EBK PLUS assay were from patients who were sent to the laboratory for HBV testing. Of those, 100 (42%) were frozen and 136 (58%) were fresh. The patients represented Florida, Georgia, Pennsylvania, California, Utah, and the southeastern US. The group was 69% (162/236) female, 29% (68/236) male and 2% (6/236) unspecified; the ethnicity of the patients was unspecified. The ages ranged from 5 to 88 years old, with 6 samples unspecified. The percent DiaSorin ETI-EBK PLUS positive results observed in these samples was 7%.

The table below summarizes the percent DiaSorin ETI-EBK PLUS positive and negative results by gender and age range. There were 6 samples for which gender and age were not reported; they were all positive. There were 6 other samples for which age was not reported, 2 were from females and 4 were from males; all were negative. These 12 results were not included in the table.

		DiaSorin ETI-EBK PLUS				
		+		-		
Age Range	Gender	n	%	n	%	TOTAL
0-9	F	0	0%	2	100%	2
	M	0	NA	0	NA	0
10-19	F	1	6%	16	94%	17
	M	1	50%	1	50%	2
20-29	F	1	2%	50	98%	51
	M	3	23%	10	77%	13
30-39	F	1	2%	48	98%	49
	M	1	6%	16	94%	17
40-49	F	1	5%	19	95%	20
	M	1	7%	13	93%	14
50-59	F	4	80%	1	20%	5
	M	1	13%	7	88%	8
60-69	F	0	0%	3	100%	3
	M	0	0%	2	100%	2
70-79	F	0	0%	10	100%	10
	M	0	0%	5	100%	5
80-89	F	0	0%	3	100%	3
	M	0	0%	3	100%	3
TOTAL		15	7%	209	93%	224


Acute Serial Panels

One hundred twenty-four (124) archived serial samples from 9 individuals were analyzed. Most (8/9) of these individuals were defined as being acutely infected by the appearance of HBsAg and HBeAg with the subsequent appearance of IgM aHBc, total HBc, aHBe, and aHBs. One individual had detectable HBsAg but did not have detectable HBeAg in any specimen. However, this individual did seroconvert for aHBe.

The specimens were collected from individuals undergoing plasmaphereses for further manufacturing purposes. Three individuals were found to be infected with HBV during the first plasmaphereses and others became infected with HBV during subsequent plasmaphereses. It is unknown how long these three initially HBsAg reactives were infected prior to the first plasmapheresis. All nine individuals underwent sequential plasmaphereses after becoming HBV infected. However, the timing of subsequent plasmaphereses varied from individual to individual. The specimens draw times were normalized to represent the day that HBsAg was first detected by an FDA licensed assay as Day 0. For the remaining specimens, draw days ranged from day 0 (HBsAg first detected) through day 355 post day 0. Since all panels did not contain the same draw day, sample results were grouped within day intervals (e.g. days 0, 1-10, 11-20, etc., representing days since first detection of HBsAg).

The results are summarized in the following table and graph. No specimen was reactive for HBeAg by the DiaSorin assay after day 90. In the graph below the graph for the reference HBsAg percent reactive has been overlaid for reference.

Day Range	Number Specimens	DiaSorin HBeAg Reactive	% Positive
0	9	1	11.1
1-10	10	5	50.0
11-20	13	10	76.9
21-30	9	6	66.7
31-40	10	7	70.0
41-50	6	1	16.7
51-60	10	2	20.0
61-70	9	3	33.3
71-80	6	2	33.3
81-90	9	1	11.1
91-100	10	0	NA
101-110	6	0	NA
111-120	4	0	NA
121-130	4	0	NA
131-140	3	0	NA
141-150	2	0	NA
151-160	0	0	NA
161-170	1	0	NA
171-180	0	0	NA
181-190	1	0	NA
191-200	1	0	NA
355	1	0	NA

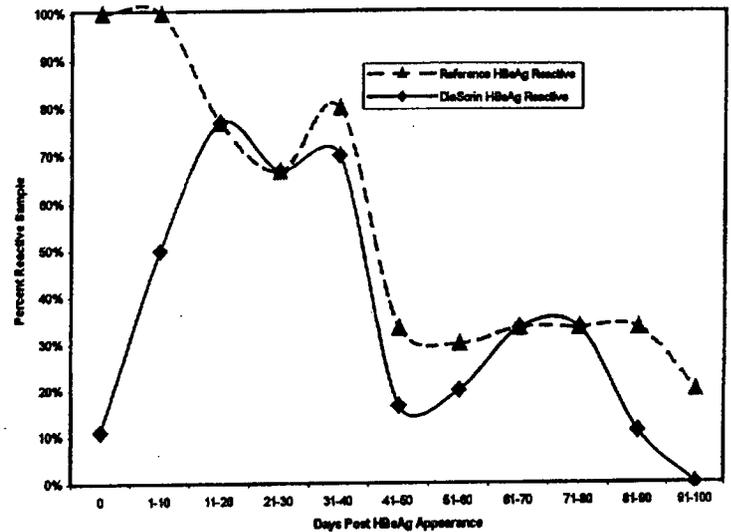

16. PERFORMANCE DATA

Clinical Samples

Since the majority of studies were performed on pre-selected retrospective specimens, no calculations for the assay's positive and negative predictive values may be performed or inferred.

Prospective Samples: A study of 136 prospective specimens was conducted. These specimens represented individuals who were sent to the laboratory for hepatitis testing. Specimens were collected at a reference laboratory and assayed at the California clinical trial site. The patients were 86% (117/136) female and 14% (19/136) male. The ages ranged from 5 to 77 years old, with 3 specimens not specified.

The study (testing) sites were blinded to the previous specimen categorization. All testing was performed by the manual ETI-EBK PLUS procedure. Specimens were characterized by testing with six HBV serological markers (HBsAg, HBeAg, IgM anti-HBc, total anti-HBc, anti-HBe, anti-HBs) using FDA-licensed or approved assays. Testing with these assays followed the FDA-licensed or approved procedure, including confirmation by neutralization of repeatably reactive HBsAg samples.

Results by Specimen Classification:

After study completion all samples were assigned a specimen classification based on the patterns of the six HBV serological markers established by the reference assays. Based on these serological marker patterns, the samples were categorized into the HBV classifications described in the table below. There were 6 unique HBV marker patterns observed in the DiaSorin ETI-EBK PLUS prospective clinical studies.

Characterization Based On Single Point Specimen	HBsAg	HBeAg	IgM anti-HBc	Total anti-HBc	anti-HBe	anti-HBs	n
Chronic Infection	+	-	-	+	+	-	1
Recovery	-	-	-	+	+	+	2
Past Infection	-	-	-	+	-	+	4
	-	-	-	+	-	-	4
HBV Vaccine Response	-	-	-	-	-	+	38
Not Previously Infected with HBV	-	-	-	-	-	-	87

Based on the above classifications the DiaSorin HBeAg results for the prospective samples were compared to a reference assay's HBeAg results. The following table shows this comparison and percent agreement with 95% confidence intervals with the reference HBeAg assay.

Prospective Samples Comparison

Reference Serology Classification	-	Reference HBeAg
	-	DiaSorin HBeAg
Chronic infection	1	1
Recovery	2	2
Past Infection	8	8
HBV vaccine response	38	38
Not previously infected with HBV	87	87
Grand Total	136	136

Prospective Samples:

Chronic Infection	Positive agreement with reference assay results = N/A (0/0) 95% CI = N/A
	Negative agreement with reference assay results = 100% (1/1) 95% CI = 2.5 to 100%
Recovery	Positive agreement with reference assay results = N/A (0/0) 95% CI = N/A
	Negative agreement with reference assay results = 100.0% (2/2) 95% CI = 15.8 to 100.0%
HBV Vaccine Response	Positive agreement with reference assay results = NA (0/0) 95% CI = NA
	Negative agreement with reference assay results = 100% (38/38) 95% CI = 90.8 to 100%
Past Infection	Positive agreement with reference assay results = NA (0/0) 95% CI = NA
	Negative agreement with reference assay results = 100% (8/8) 95% CI = 63.1 to 100%
Not Previously Infected	Positive agreement with reference assay results = NA (0/0) 95% CI = NA
	Negative agreement with reference assay results = 100% (87/87) 95% CI = 98.5 to 100%

Retrospective Samples: Retrospective studies were carried out at three clinical laboratories in the United States (California, Missouri, and Minnesota) and at DiaSorin (Italy) to assess the performance of the ETI-EBK PLUS assay in detecting HBeAg. The study set included 650 frozen repository samples (the majority of which were purchased from commercial vendors) from the following populations:

- patients with chronic hepatitis B infection (diagnosed by a physician as having HBsAg positive for greater than 6 months) – 111 frozen repository samples;
- patients with serologically diagnosed hepatitis B infection (acute, chronic, asymptomatic, convalescent, etc.) – 82 frozen repository samples;
- patients sent to the laboratory for hepatitis B testing – 100 frozen repository samples;
- a general hospital patient population – 357 frozen repository samples.

The specimens represented Midwestern (2%), Southeastern (25%), Western (13%), and Northeastern US (2%), outside of the US (1%), and unspecified (57%). The group was 44% (287/650) female, 42% (270/650) male, and 14% (93/650) unspecified. Approximately 13% (84/650) were Caucasian, 4% (27/650) were African American, <1% (5/650) were Hispanic, <1% (3/650) were Asian, and 82% (531/650) were unspecified. The ages ranged from 5 to 98 years old, with 131 specimens not specified.

The study (testing) sites were blinded to the previous specimen categorization. All testing was performed by the manual ETI-EBK PLUS procedure. Specimens were characterized by testing with six HBV serological markers (HBsAg, HBeAg, IgM anti-HBc, total anti-HBc, anti-HBe, anti-HBs) using FDA-licensed or approved assays. Testing with these assays followed the FDA-licensed or approved procedure with the exception of the HBsAg assay at two of the three sites. At these sites, the majority of specimens that were initially HBsAg-positive were repeated in duplicate, however the repeatedly reactive specimens were not confirmed by the licensed HBsAg confirmation assay at the two sites. Therefore, true HBsAg result was determined in one of three ways: 1) confirmed by reference assay neutralization during clinical trials, 2) based on a statement by the attending physician that HBsAg was positive for greater than 6 months, or 3) information provided by the vendor regarding confirmatory testing performed at their location or by the material source facility.

Results by Specimen Classification:

After study completion all samples were assigned a specimen classification based on the patterns of the six HBV serological markers established by the reference assays. Based on these serological marker patterns, the samples were categorized into the HBV classifications described in the table below. There were 35 unique HBV marker patterns observed in the DiaSorin ETI-EBK PLUS retrospective clinical studies.

Characterization Based On Single Point Specimen	HBsAg	HBeAg	IgM anti-HBc	Total anti-HBc	anti-HBe	anti-HBs	n
Acute infection	+	+	+ or I	+	-	-	52
	+	-	+ or I	+	+	-	4
	+	-	-	-	-	-	2
	+	+	-	-	-	-	2
Chronic Infection	+	-	-	+	+	-	82
	+	+	-	+	-	-	21
	+	-	-	+	- or I	-	23
	+	+	+	+	-	+	4
	+	+	- or I	+	-	+	2
	+	-	-	+	+	+	2
	+	+	-	+	+ or I	+	2
	+	+	+	+	+	+	1
	+	+	-	+	+	-	1

Characterization Based On Single Point Specimen	HBsAg	HBeAg	IgM anti-HBc	Total anti-HBc	anti-HBe	anti-HBs	n
	+	-	-	+	-	+	1
Recovery	-	-	-	+	+ or I	+	40
	-	-	-	+	+	-	6
	-	-	+	+	+	-	2
	-	-	+ or I	+	+	+	2
Past Infection	-	- or I	-	+	-	+	12
	-	-	-	+	-	-	9
HBV Vaccine Response	-	-	-	-	-	+	20
Not Previously Infected with HBV	-	-	-	-	-	-	343
Uninterpretable	-	+ or I	-	-	-	-	13
	-	+	-	+	-	+	2
	-	+	-	+	+	+	1
	-	I	-	+	-	-	1

*I = indeterminate result

Based on the above classifications the ETI-EBK PLUS HBeAg results for the retrospective samples were compared to a reference assay's HBeAg results as determined by the methods above. The following table shows this comparison and percent agreement with 95% confidence intervals with the reference HBeAg results.

Retrospective Samples Comparison

Reference Serology Classification	-		+		I [†]	Reference HBeAg
	-	+	-	+	-	DiaSorin HBeAg
Acute infection	5	1	0	54	0	60
Chronic infection	107	1	2	29	0	139
Recovery	50	0	0	0	0	50
HBV vaccine response	20	0	0	0	0	20
Not previously infected with HBV	343	0	0	0	0	343
Past Infection	20	0	0	0	1	21
Uninterpretable	0	0	9	1	7	17
Total	545	2	11	84	8	650

[†] Indeterminate result

Retrospective Samples:

Acute Infection

Positive agreement with reference assay results = 100% (54/54)

95% CI = 93.4 to 100%

Negative agreement with reference assay results = 83.3% (5/6)

95% CI = 35.9 to 99.6%

Chronic Infection

Positive agreement with reference assay results = 93.5% (29/31)

95% CI = 78.6 to 99.2%

Negative agreement with reference assay results = 99.1% (107/108)

95% CI = 95.0 to 100%

Recovery

Positive agreement with reference assay results = NA (0/0)

95% CI = NA

Negative agreement with reference assay results = 100% (50/50)

95% CI = 92.9 to 100.0%

HBV Vaccine Response

Positive agreement with reference assay results = NA (0/0)
95% CI = NA
Negative agreement with reference assay results = 100% (20/20)
95% CI = 83.2 to 100.0%

Not Previously Infected

Positive agreement with reference assay results = NA (0/0)
95% CI = NA
Negative agreement with reference assay results = 100% (343/343)
95% CI = 98.9 to 100%

Past Infection

Positive agreement with reference assay results = NA (0/0)
95% CI = NA
Negative agreement with reference assay results = 100% (20/20)
95% CI = 83.2 to 100%


Uninterpretable

Positive agreement with reference assay results = 10.0% (1/10)
95% CI = 0.3 to 44.5%
Negative agreement with reference assay results = NA (0/0)
95% CI = NA

Instrument Comparison of Biochem Immunosystems Labotech/ETI-LAB to the Manual Method: An instrument application study was conducted at DiaSorin, Saluggia Italy, to evaluate the performance of the ETI-EBK PLUS assay on the Biochem Immunosystems Labotech/ETI-LAB, an automated microplate processing instrument, compared to the manual analysis. The Paul Ehrlich-Institut (PEI) Standard, 12 serum samples near the ETI-EBK PLUS cutoff and samples from the clinical trials (29 suspected hepatitis B patients and 11 apparently healthy adults) were tested in parallel manually and on the Labotech.

Serial dilutions of the PEI Standard were prepared in fetal calf serum to obtain a panel ranging from high concentration to below the analytical sensitivity of the assay. The diluted Standard samples were tested in duplicate, one run per day for three days both manually and on the Labotech. Due to the requirement that assay cutoff be established for each plate, reproducibility was evaluated based on specimen absorbance-to-cutoff ratios (S/CO) rather than absolute absorbance values. The 95% confidence intervals were established for the S/CO values of each point of the Standard-referenced curve and therefore the analytical endpoint sensitivity was defined (first dilution with S/CO > 1.1). A graph summarizing these results is presented below:

INSTRUMENT APPLICATION STUDY: PEI curve
ETI-EBK PLUS

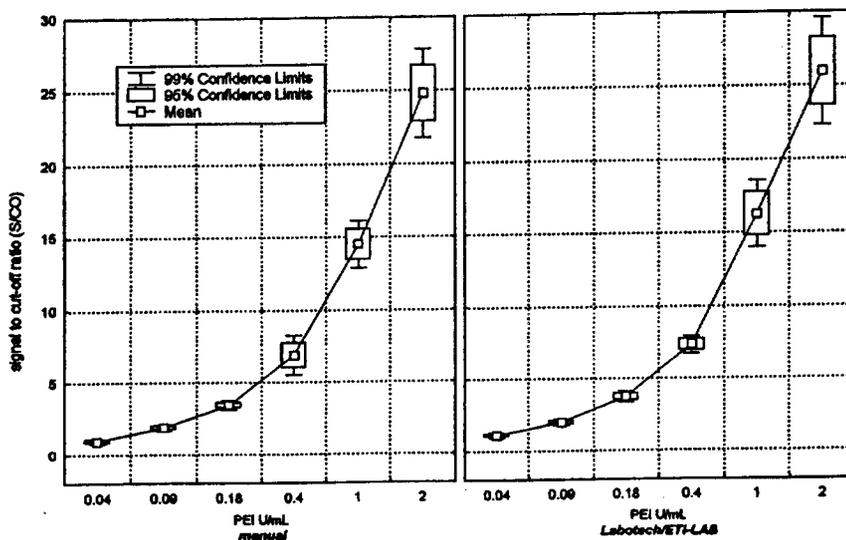

The 12 samples near the cutoff were tested in triplicate, one run per day for three days both manually and on the Labotech. The samples from the clinical trials were tested in singlet in one run on one day, both manually and on Labotech. The mean, the standard deviation and the coefficient of variation (CV%) of the S/CO values were computed by the different components of variability for each of the tested specimens. A summary of the data is presented in the following table.

Analytical Endpoint Sensitivity (0.18 PEI U/mL)	Manual			Labotech/ETI-LAB		
	Mean	W/R %CV ^a	D/D %CV	Mean	W/R %CV	D/D %CV
S/CO [95% CI] ^b	1.87 [1.75 – 1.99]	4.2	5.8	1.97 [1.82 – 2.13]	4.0	7.2
12 Cutoff Samples S/CO Range of mean	0.96 0.74 – 1.11	7.1	5.8	1.09 0.84 – 1.27	5.0	3.7
Clinical Samples:						
Suspected Hepatitis B Range of S/CO	Negative: 0.00 – 0.50 (8/29) Equivocal: 0.94 (1/29) Positive: 6.46 – >51 (20/29)			Negative: 0.06 – 0.71 (8/29) Equivocal: N/A (0/29) Positive: 1.15 – >45 (21/29)		
Healthy Adults Range of S/CO	Negative: -0.05 – 0.43 (11/11) Equivocal: N/A (0/11) Positive: N/A (0/11)			Negative: 0.09 – 0.44 (11/11) Equivocal: N/A (0/11) Positive: N/A (0/11)		

^a %CVs were calculated using specimen absorbance-to-cutoff ratios (S/CO) which normalized the data plate-to-plate

^b 95% CI = 95% Confidence Interval; W/R = within-run; D/D = day-to-day

Reproducibility

Manual Assay: Intra-assay, inter-assay, inter-lot, and inter-site variability studies were carried out on the ETI-EBK PLUS kit to test the variability within runs, between runs, between days, between kit lots, and between test sites. Variability was measured on a panel of ten sera that included negative, borderline, and positive samples. Three ETI-EBK PLUS kit lots were tested at three independent test sites. Due to the requirement that assay cutoff be established for each plate, reproducibility was evaluated based on specimen absorbance to cutoff ratios (S/CO) rather than absolute absorbance values. The results of that study are tabulated below.

Clinical Site Reproducibility

ID#		# of Tests per Sample	Mean S/CO's	Within-run %CV*	Between-run %CV	Between-lot %CV	Between-day %CV	Between-site %CV	Total
S01	High	108	20.03	6.37	6.29	10.07	7.30	5.14	14.47
S02	High	108	10.83	4.16	5.07	11.56	7.34	9.44	15.69
S03	High	108	6.83	4.47	7.16	11.78	7.09	6.73	17.18
S04	Low	108	3.84	3.80	8.25	14.42	6.97	5.79	17.12
S05	Equiv	108	0.80	6.08	6.79	8.51	6.38	3.79	13.03
S06	Low	108	2.61	5.35	5.99	9.72	7.92	9.80	14.35
S07	Low	108	2.11	3.55	10.49	10.44	7.47	10.18	17.97
S08	Low	108	1.96	5.08	11.86	10.47	6.86	7.30	16.18
S09	Equiv	108	1.67	6.27	11.85	10.47	4.04	4.04	19.19
S10	Neg	108	0.06	20.20	36.73	36.18	15.26	29.61	89.32

* %CVs were calculated using specimen absorbance-to-cutoff ratios (S/CO) which normalized the data plate-to-plate

Plasma Reproducibility: A plasma reproducibility study was conducted at DiaSorin, Saluggia Italy, to evaluate the performance of the manual ETI-EBK PLUS assay on serum versus a variety of plasma types. The plasma types evaluated were citrate, heparin and EDTA. Sample sets of matched serum/multiple plasma were used in the study. A sample set was prepared by spiking the same high positive sample into each of the matrices (serum and plasmas) resulting in a total of four specimens per set around the cutoff. Several high positive samples were used in the preparation of the 12 different near-cutoff sample sets. Six matched serum/multiple plasma samples sets were tested in triplicate in each run; thus there were two runs per day for three days, all tested in a manual mode. Due to the requirement that assay cutoff be established for each plate, reproducibility was evaluated based on specimen absorbance to cutoff ratios (S/CO) rather than absolute absorbance values. The mean, the standard deviation and the coefficient of variation (CV%) of the S/CO values were computed by the different components of variability for each of the tested specimens. The 95% confidence intervals were established for the S/CO values of all serum samples and each plasma type. A summary of the data is presented in the following table.

	SERUM	CITRATE	HEPARIN	EDTA
Mean (S/CO)	0.99	0.99	1.02	1.04
95% CI*	0.95 - 1.03	0.95 - 1.03	0.98 - 1.06	1.00 - 1.08
W/R %CV**	5.9%	4.8%	5.4%	4.5%
D/D %CV	9.3%	7.7%	7.2%	8.5%
Total %CV	10.4%	8.6%	8.6%	8.9%
Between matrix %CV	7.9%			
Across matrix total %CV	11.7%			

* CI = 95% Confidence Interval; W/R = within-run; D/D = day-to-day; 95%

** %CVs were calculated using specimen absorbance-to-cutoff ratios (S/CO) which normalized the data plate-to-plate

Assay reproducibility using the Labotech has not been established. If the Labotech is used, the user should establish appropriate assay reproducibility in accordance with NCCLS EP5-A, Evaluation of Precision Performance of Clinical Chemistry Devices.

Analytical Sensitivity

The analytical sensitivity of the assay (the smallest quantity of analyte that can be distinguished from background) was evaluated using single point serial dilutions of a standard preparation from the Paul-Ehrlich-Institut, Germany (PEI). The analytical sensitivity of the assay (last positive dilution) was determined to be 0.2 PEI U/mL (Mean Signal-to-Cutoff Ratio = 3.43; 95% Confidence Interval = 3.22 to 3.65).

Cross-Reactivity

Of the 525 potential interfering samples, 513 (98%) were negative and 12 (2%) were positive by ETI-EBK PLUS. Among the 12 positive samples, 4 were negative for HBsAg and IgM anti-HBc and negative for HBeAg on repeat testing; 7 were positive by reference testing or review of hepatitis B marker patterns for those samples. Disease was determined by serological testing, there is no guarantee that the associated antigen was present in the tested material. Interference testing with the described specimens was not performed.

Cross-Reactivity Study Results

GROUP	N	ETI-EBK PLUS Negative Samples	ETI-EBK PLUS Positive Samples	% Confirmed Positive By Additional Testing
Acute EBV infection	16	16	0	-
Acute CMV infection	20	20	0	-
Acute HSV infection	10	10	0	-
Acute Toxoplasma infection	18	18	0	-
Acute parvovirus B19 infection	5	5	0	-
HTLV-I/II infection	50	48	2*	-
Syphilis	26	26	0	-
HCV infection	50	50	0	-
HDV infection	20	17	3	100% (3/3)
HIV infection	50	49	1*	-
Acute HAV infection	50	49	1	0% (0/1)
Past HAV infection	50	48	2	100% (2/2)
Rheumatoid factor (RF) +	40	40	0	-
Autoimmune disease	19	19	0	-
Systemic lupus erythematosus (SLE)	11	11	0	-
Autoimmune hepatitis	5	5	0	-
Myeloma	20	19	1*	-
Hypergammaglobulinemia	20	20	0	-
Influenza vaccine	5	5	0	-
Elevated liver enzymes	10	10	0	-
Non-viral liver disease	30	28	2	100%(2/2)
TOTAL	525	513 (98%)	12 (2%)	88% (7/8)

*These samples were negative for HBsAg and IgM anti-HBc, and negative on repeat testing on ETI-EBK PLUS.

A BLAST analysis was performed to determine if untested viral or bacterial proteins could potentially cross-react with the anti-HBe monoclonal antibodies used in this assay. The only protein that showed some homology was the HB core antigen. Additional cross-reactivity studies showed that the antigen cross-reacted with the assay only when the monoclonal antibody was present at approximately 83 times the concentration used in the assay. No notable similarities in protein sequences were identified from the other viral or bacterial proteins, suggesting that they should not cross-react in this assay.

Substances That Do Not Interfere

As recommended by NCCLS Protocol EP7 (27), the DiaSorin ETI-EBK PLUS assay was evaluated for interference by testing the following substances. Testing was performed using matched pairs of negative donor serum and negative donor serum spiked with a high titer HBeAg samples to obtain a result near the cutoff. None of the compounds at the levels indicated were found to interfere with the clinical interpretation of the assay in serum. No interference was found with

bilirubin in plasma (EDTA, heparin or citrate), testing for interference with hemoglobin and triolein was not performed in plasma.

Compound	Concentration	
Bilirubin	0.35 mmol/L	20 mg/dL
Hemoglobin	0.06 mmol/L	100 mg/dL
Triolein	33.9 mmol/L	3000 mg/dL

The ETI-EBK PLUS assay was also evaluated for possible interference from heterophilic anti-mouse antibodies (HAMA). A dilutional panel was used, consisting of 21 samples prepared from a stock pool of high positive human serum. The HAMA concentrations in the samples ranged from 0 to 2975.5 ng/mL, as determined by a HAMA ELISA. In a direct non-competitive assay, such as ETI-EBK PLUS, interference would manifest as false positive results. No interference was seen in that all 21 dilutions were negative by the ETI-EBK PLUS assay, and supported by positive anti-HBe results.

17. ABBREVIATED TEST PROCEDURE

1. DISPENSE 50 µL INCUBATION BUFFER.
2. DISPENSE 100 µL CALIBRATOR, CONTROLS AND SAMPLES INTO WELLS, LEAVING AN EMPTY WELL FOR THE BLANK.
3. INCUBATE FOR TWO HOURS AT 37°C.
4. ASPIRATE THE LIQUID. WASH THE WELLS REPEATEDLY WITH WORKING WASH BUFFER.
5. DISPENSE 100 µL ENZYME TRACER TO EACH WELL.
6. INCUBATE FOR 60 MINUTES AT 37°C.
7. ASPIRATE THE LIQUID. WASH THE WELLS REPEATEDLY WITH WORKING WASH BUFFER.
8. DISPENSE 100 µL CHROMOGEN/SUBSTRATE TO EACH WELL.
9. INCUBATE FOR 30 MINUTES AT ROOM TEMPERATURE.
10. DISPENSE 100 µL STOP SOLUTION TO EACH WELL.
11. READ THE ABSORBANCE VALUES WITH A PHOTOMETER AT 450/630 nm WITHIN 60 MINUTES.

18. REFERENCES

1. Escobar MR: Chronic viral hepatitis, in Specter S, Lancz GJ (eds): *Clinical Virology Manual*. New York, Elsevier, 1986, pp 329-348.
2. Lee HS, Vyas GN: Diagnosis of viral hepatitis. *Clin Lab Med* 1987; 7: 741-757.
3. Hirschman SZ: Hepatitis viruses and Viral hepatitis, in Braude AI, Davis CE, Fierer J (eds): *Infectious Diseases and Medical Microbiology*, ed 2. Philadelphia, WB Saunders, 1986, pp 557-564; 989-995.
4. Szmunes W: Recent advances in the study of the epidemiology of hepatitis B. *Am J Pathol* 1975; 81 (3): 629-650.

5. Mast EE, Alter HJ: Epidemiology of viral hepatitis: an overview. *Sem in Virol* 1993; 4: 273-283.
6. Christie AB: *Infectious Diseases: epidemiology and clinical practice*. London, Churchill Livingstone, 1980, pp 447-518.
7. *Morbidity and Mortality Weekly Report*. Centers for Disease Control and Prevention (CDC), Atlanta, Georgia, 1995, pp. 43-53.
8. Feitelson MA: Biology of hepatitis B virus variants. *Lab Invest* 1994; 71 (3): 324.
9. Heermann KH et al: Large surface proteins of hepatitis B virus containing the pre-S sequence. *J Virol* 1984; 52 (2): 396-402.
10. Norder H et al: Comparison of the amino acid sequences of nine different serotypes of hepatitis B surface antigen and genomic classification of the corresponding hepatitis B virus strain. *J Gen Virol* 1992; 73: 1201-1208.
11. Gerlich WH et al: Specificity and localization of the hepatitis B virus-associated protein kinase. *J Virol* 1982; 42 (3): 761-766.
12. Cohen BJ, Richmond JE: Electron microscopy of hepatitis B core antigen synthesized in *E. coli*. *Nature* 1982; 296 (5858): 677-679.
13. Milich DR, McLachlan A: The nucleocapsid of hepatitis B virus is both a T-cell-independent and a T-cell-dependent antigen. *Science* 1986; 234 (4782): 1398-1401.
14. Schlicht HJ, Salfeld J, Schaller H: The duck hepatitis B virus pre-C region encodes a signal sequence which is essential for synthesis and secretion of processed core proteins but not for virus formation. *J Virol* 1987; 61 (12): 3701-3709.
15. Gerlich W, Thomssen R: Terminology, structure and laboratory diagnosis of hepatitis viruses, in McIntyre N et al (eds): *Oxford Textbook of Clinical Hepatology*. Oxford University Press, 1991, pp. 543-560.
16. Moradpour D, Wands JR: Understanding hepatitis B virus infection: *N E J Med* 1995; 332: 1092.
17. Dusheiko G, Hoofnagle JH: Hepatitis B, in McIntyre N et al (eds): *Oxford Textbook of Clinical Hepatology*. Oxford University Press, 1991, pp. 571-577.
18. Chen DS, Lai MY, Lee SC et al: Serum HBsAg, HBeAg, anti-HBe, and hepatitis B viral DNA in asymptomatic carriers in Taiwan. *J Med Virol* 1986; 19: 87-94.
19. Carman WF et al: Mutation preventing formation of HBeAg in patients with chronic HBV infection. *Lancet* 1989; 2: 588-591.
20. *Biosafety in Microbiological and Biomedical Laboratories*, Richardson JH, Barkley WE (eds). Atlanta, GA, US Dept of Health and Human Services, Public Health Service, Centers for Disease Control; Bethesda, MD, National Institutes of Health, 3rd ed., 1993. HHS Publication No. (CDC) 93-8395.
21. *Occupational Exposure to Bloodborne Pathogens; Final Rule*. Federal Register. Part II; Department of Labor, Occupational Safety and Health Administration (OSHA); 29 CFR Part 1910.1030; Friday, December 6, 1991.
22. *National Committee for Clinical Laboratory Standards. Protection of laboratory workers from infectious disease transmitted by blood and tissue; Tentative Guideline*, 2nd ed. NCCLS Document M29-T2. Villanova, PA; NCCLS: 1991.

23. National Committee for Clinical Laboratory Standards. Procedure for the Handling and Processing of Blood Specimens; Approved Guideline, 2nd Edition. NCCLS Document H18-A2. Villanova, PA; NCCLS: 1999.
24. U.S. Public Health Services, HHS 1996. Code of Federal Regulations Title 42 Part 72 - Interstate shipment of etiologic agents. U.S. Government Printing Office, Washington, D.C.
25. Westgard JO, Barry PL: Cost-effective Quality Control: managing the quality and productivity of analytical processes. Washington, D.C., AACC Press, 1986.
26. National Committee for Clinical Laboratory Standards. Internal Quality Control Testing: principles and definition; Approved Guideline. NCCLS Document C24-A. Villanova, PA; NCCLS: 1991.
27. National Committee for Clinical Laboratory Standards. Interference Testing in Clinical Chemistry; Proposed Guideline. NCCLS Document EP7-A. Villanova, PA; NCCLS: 1986.