



Food and Drug Administration
10903 New Hampshire Avenue
Document Control Room -WO66-G609
Silver Spring, MD 20993-0002

Mr. George Papagiannis, M.Eng.
Quality Assurance and Regulatory Affairs
Stellate Systems
345 Victoria Avenue, Suite 300
Canada H3Z 2N2

APR - 9 2012

Re: K013450
Trade/Device Name: Notta Ambulatory Recorder
Regulation Number: 21 CFR 882.1400
Regulation Name: Electroencephalograph
Regulatory Class: II
Product Code: OLV, GWQ
Dated (Date on orig SE ltr): October 9, 2001
Received (Date on orig SE ltr): October 17, 2001

Dear Mr. Papagiannis:

This letter corrects our substantially equivalent letter of January 14, 2002.

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

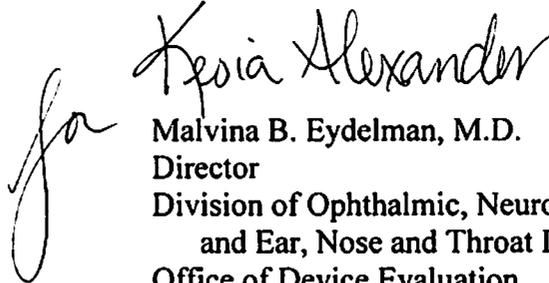
If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); medical device reporting (reporting of medical device-related adverse events) (21 CFR 803); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please go to <http://www.fda.gov/AboutFDA/CentersOffices/CDRH/CDRHOFFices/ucm115809.htm> for the Center for Devices and Radiological Health's (CDRH's) Office of Compliance. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to <http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/default.htm> for the CDRH's Office of Surveillance and Biometrics/Division of Postmarket Surveillance.

You may obtain other general information on your responsibilities under the Act from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 796-7100 or at its Internet address <http://www.fda.gov/MedicalDevices/ResourcesforYou/Industry/default.htm>.

Sincerely yours,

A handwritten signature in black ink, appearing to read "Malvina B. Eydelman". The signature is written in a cursive style with a large, stylized initial "M".

Malvina B. Eydelman, M.D.
Director
Division of Ophthalmic, Neurological,
and Ear, Nose and Throat Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

Attachment A

Indications for Use Statement

510(k) Number: K 013450

Device Name: **Notta Ambulatory Recorder**

Indications for Use:

The Notta Ambulatory Recorder is indicated for the recording and study of EEG and other physiological signals obtained during routine EEG exams, long-term monitoring in epilepsy (LTM) and sleep studies (PSG or polysomnography) either at home, at a clinical setting, or other suitable environment under physician's order.

The Notta Ambulatory Recorder is indicated for use with children and adults under the supervision of a physician or other trained health care professional. The device is intended to be worn by the patient during a recording session.

The Notta Ambulatory Recorder is not intended to be used for the monitoring of vital signs, in critical care or intra-operative settings.

In no way are any of the device functions represented as being in and of themselves diagnostic. The system requires competent user input, and its output must be reviewed and interpreted by a physician or other trained health care professional who will exercise professional judgment in using this information.

PLEASE DO NOT WRITE BELOW THIS LINE - CONTINUE ON ANOTHER PAGE IF NEEDED

f Mark N. Miller
(Division Sign-Off)
Division of General, Restorative
and Neurological Devices

Concurrence of CDRH, Office of Device Evaluation (ODE)

510(k) Number K013450

Prescription Use
(Per 21 CFR 801.109)

OR Over-The-Counter Use