

SEP 2 1999

510(k) SUMMARY

Submitter's Name: Guidant Corporation
Advanced Cardiovascular Systems, Inc.
Submitter's Address: 3200 Lakeside Drive
Santa Clara, CA 95052
Telephone: 408-235-3000
Fax: 408-235-3743
Contact Person: Sandra Sundell
Date Prepared: March 15, 1999

Device Trade Name: RX HERCULINK™ 14 Biliary Stent System

Device Common Name: Biliary stent

Device Classification Name: Biliary Catheter

Device Classification: Class II

Summary of Substantial Equivalence:

The design, materials, method of delivery and intended use features of RX HERCULINK™ 14 Biliary Stent System are substantially equivalent with regard to these features in the predicate device, the Cordis J&J PALMAZ™ balloon-expandable Stent and delivery catheter for the Biliary System (K911581).

Device Description:

RX HERCULINK™ 14 Biliary Stent System is a balloon-expandable stent pre-mounted onto a rapid exchange (RX) delivery catheter designed to be placed percutaneously into the common bile duct and intended to treat malignant strictures in the biliary tree. The stent is fabricated from a single piece of 316L medical grade stainless steel tubing. The stent is pre-mounted onto an RX delivery catheter with an integrated shaft system and an XCELON™ (nylon blend) balloon bonded at the distal end. The shaft has a combination of a single lumen design at the proximal end and a coaxial lumen at the distal end. The proximal lumen provides for inflation of the balloon with contrast medium. The distal lumen permits use of a guide wire to facilitate advancement of the catheter to and through the stenosis to be dilated.

The balloon, which has 2 radiopaque markers to aid in positioning the balloon in the stenosis, is designed to provide an expandable segment of known diameter and length at specific pressures.

The proximal end of the catheter has a single arm adapter that provides access to the inflation lumen. It is designed with a luer-lock fitting for connection with an inflation device.

The RX HERCULINK™ Biliary Stent System consists of an 18 mm length stent pre-mounted onto a 75 cm length delivery catheter with balloon diameters of 4.0, 4.5, 5.0, 5.5, 6.0, 6.5 and 7.0 mm. The RX HERCULINK™ 14 Biliary Stent System is intended to be delivered and deployed in the biliary tree.

Intended Use:

The RX HERCULINK™ 14 Biliary Stent System is indicated for palliation of malignant strictures in the biliary tree.

Technological Characteristics:

The RX HERCULINK™ 14 Biliary Stent System incorporates similar design, components, method of deployment, materials and intended use of the predicate device, Cordis J&J PALMAZ™ balloon-expandable Stent and delivery catheter for the Biliary System (K911581). The RX HERCULINK™ 14 Biliary Stent System consists of an 18 mm length stent pre-mounted onto a 75 cm length delivery catheter with balloon diameters of 4.0, 4.5, 5.0, 5.5, 6.0, 6.5 and 7.0 mm.

Performance Data:

The safety and effectiveness of the RX HERCULINK™ 14 Biliary Stent System has been demonstrated through data collected from *in vitro* bench tests and analyses.



Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

SEP 2 1999

Ms. Sandra Sundell
Senior Regulatory Affairs Coordinator
Guidant Corporation
Advanced Cardiovascular Systems
P.O. Box 58167
Santa Clara, California 95052-8167

Re: K990867
RX HERCULINK™ 14 Biliary Stent System
Regulatory Class: II
21 CFR 876.5010
Product Code: 78 FGE
Dated: July 1, 1999
Received: July 2, 1999

Dear Ms. Sundell:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act and the limitations described below. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

The Office of Device Evaluation has determined that there is a reasonable likelihood that this device will be used for an intended use not identified in the proposed labeling and that such use could cause harm. Therefore, in accordance with Section 513(i)(1)(E) of the Act, the following limitation must appear in the Warnings section of the device's labeling:

The safety and effectiveness of this device for use in the vascular system have not been established.

Furthermore, the indication for biliary use must be prominently displayed in all labeling, including pouch, box, and carton labels, instructions for use, and other promotional materials, in close proximity to the trade name, of a similar point size, and in bold print.

Page 2 – Ms. Sandra Sundell


If your device is classified (see above) into either class II (Special Controls) or class III (Pre-market Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the Current Good Manufacturing Practice requirements, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic QS inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. *Please note:* this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and permits your device to proceed to the market. This letter will allow you to begin marketing your device as described in your 510(k) premarket notification if the limitation statement above is added to your labeling, as described.

Please note that the above labeling limitations are required by Section 513(i)(1)(E) of the Act. Therefore, a new 510(k) is required before these limitations are modified in any way or removed from the device's labeling.

If you desire specific information about the application of other labeling requirements to your device (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4616. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its Internet address "<http://www.fda.gov/cdrh/dsma/dsmamain.html>".

Sincerely yours,

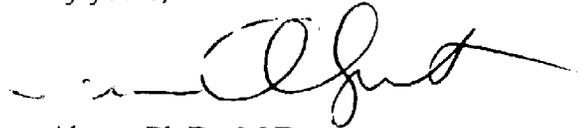

Susan Alpert, Ph.D., M.D.
Director
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

510(k) Number (if known): K990867

Device Name: RX Herculink™ 14 Biliary Stent System

FDA's Statement of the Indications For Use for device:

The RX Herculink™ 14 Biliary Stent System is indicated for the palliation of malignant neoplasms in the biliary tree.

Prescription Use OR Over-The-Counter Use
(Per 21 CFR 801.109)



(Division Sign-Off)
Division of Reproductive, Abdominal, ENT,
and Radiological Devices
510(k) Number K990867 / S^{one}