

**INFORMATION FOR THE PATIENT
3 ML DISPOSABLE INSULIN DELIVERY DEVICE**

**HUMULIN[®] 70/30 Pen
70% HUMAN INSULIN
ISOPHANE SUSPENSION
AND
30% HUMAN INSULIN INJECTION
(rDNA ORIGIN)
100 UNITS PER ML (U-100)**

WARNINGS

THIS LILLY HUMAN INSULIN PRODUCT DIFFERS FROM ANIMAL-SOURCE INSULINS BECAUSE IT IS STRUCTURALLY IDENTICAL TO THE INSULIN PRODUCED BY YOUR BODY’S PANCREAS AND BECAUSE OF ITS UNIQUE MANUFACTURING PROCESS.

ANY CHANGE OF INSULIN SHOULD BE MADE CAUTIOUSLY AND ONLY UNDER MEDICAL SUPERVISION. CHANGES IN STRENGTH, MANUFACTURER, TYPE (E.G., REGULAR, NPH, LENTE, ETC), SPECIES (BEEF, PORK, BEEF-PORK, HUMAN), OR METHOD OF MANUFACTURE (rDNA VERSUS ANIMAL-SOURCE INSULIN) MAY RESULT IN THE NEED FOR A CHANGE IN DOSAGE.

SOME PATIENTS TAKING HUMULIN[®] (HUMAN INSULIN, rDNA ORIGIN) MAY REQUIRE A CHANGE IN DOSAGE FROM THAT USED WITH ANIMAL-SOURCE INSULINS. IF AN ADJUSTMENT IS NEEDED, IT MAY OCCUR WITH THE FIRST DOSE OR DURING THE FIRST SEVERAL WEEKS OR MONTHS.

TO OBTAIN AN ACCURATE DOSE, CAREFULLY READ AND FOLLOW THE “DISPOSABLE INSULIN DELIVERY DEVICE USER MANUAL” AND THIS “INFORMATION FOR THE PATIENT” INSERT BEFORE USING THIS PRODUCT.

BEFORE EACH INJECTION, YOU SHOULD PRIME THE PEN, A NECESSARY STEP TO MAKE SURE THE PEN IS READY TO DOSE. PRIMING THE PEN IS IMPORTANT TO CONFIRM THAT INSULIN COMES OUT WHEN YOU PUSH THE INJECTION BUTTON AND TO REMOVE AIR THAT MAY COLLECT IN THE INSULIN CARTRIDGE DURING NORMAL USE. IF YOU DO NOT PRIME, YOU MAY RECEIVE TOO MUCH OR TOO LITTLE INSULIN (see also INSTRUCTIONS FOR INSULIN PEN USE section).

DIABETES

Insulin is a hormone produced by the pancreas, a large gland that lies near the stomach. This hormone is necessary for the body’s correct use of food, especially sugar. Diabetes occurs when the pancreas does not make enough insulin to meet your body’s needs.

To control your diabetes, your doctor has prescribed injections of insulin products to keep your blood glucose at a near-normal level. You have been instructed to test your blood and/or your urine regularly for glucose. Studies have shown that some chronic complications of diabetes such as eye disease, kidney disease, and nerve disease can be significantly reduced if the blood sugar is maintained as close to normal as possible. The American Diabetes Association recommends that if your pre-meal glucose levels are consistently above 130 mg/dL or your hemoglobin A_{1c} (HbA_{1c}) is more than 7%, consult your doctor. A change in your diabetes therapy may be needed. If your

46 blood tests consistently show below-normal glucose levels, you should also let your doctor know.
47 Proper control of your diabetes requires close and constant cooperation with your doctor. Despite
48 diabetes, you can lead an active and healthy life if you eat a balanced diet, exercise regularly, and
49 take your insulin injections as prescribed.

50 Always keep an extra supply of insulin as well as a spare syringe and needle on hand. Always
51 wear diabetic identification so that appropriate treatment can be given if complications occur
52 away from home.

70/30 HUMAN INSULIN

Description

55 Humulin is synthesized in a non-disease-producing special laboratory strain of *Escherichia coli*
56 bacteria that has been genetically altered by the addition of the human gene for insulin production.
57 Humulin[®] 70/30 is a mixture of 70% Human Insulin Isophane Suspension and 30% Human Insulin
58 Injection, (rDNA origin). It is an intermediate-acting insulin combined with the more rapid onset
59 of action of regular insulin. The duration of activity may last up to 24 hours following injection.
60 The time course of action of any insulin may vary considerably in different individuals or at
61 different times in the same individual. As with all insulin preparations, the duration of action of
62 Humulin 70/30 is dependent on dose, site of injection, blood supply, temperature, and physical
63 activity. Humulin 70/30 is a sterile suspension and is for subcutaneous injection only. It should not
64 be used intravenously or intramuscularly. The concentration of Humulin 70/30 in the
65 Humulin 70/30 Pen is 100 units/mL (U-100).


Identification

67 Humulin disposable insulin delivery devices, by Eli Lilly and Company, are available in
68 2 formulations — NPH and 70/30.


69 Your doctor has prescribed the type of insulin that he/she believes is best for you. **DO NOT**
70 **USE ANY OTHER INSULIN EXCEPT ON HIS/HER ADVICE AND DIRECTION.**

71 The Humulin 70/30 Pen is available in boxes of 5 disposable insulin delivery devices (“insulin
72 Pens”). The Humulin 70/30 Pen is not designed to allow any other insulin to be mixed in its
73 cartridge, or for the cartridge to be removed.

74 Always examine the appearance of Humulin 70/30 suspension in the insulin Pen before
75 administering a dose. A cartridge of Humulin 70/30 contains a small glass bead to assist in mixing.
76 Humulin 70/30 Pen must be rolled between the palms 10 times and inverted 180° 10 times before
77 each injection so that the contents are uniformly mixed (*see* Figures 1 and 2). Inspect the
78 Humulin 70/30 suspension for uniform mixing and repeat the above steps as necessary.

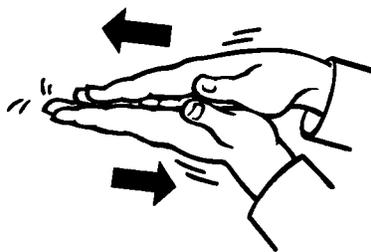

79 Figure 1.

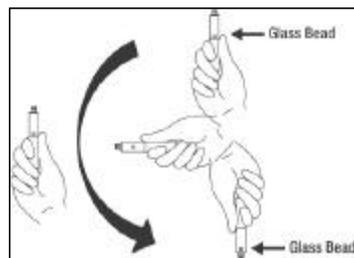

80 Figure 2.

81 Humulin 70/30 should look uniformly cloudy or milky after mixing. Do not use if the insulin
82 substance (the white material) remains visibly separated from the liquid after mixing. Do not use
83 the Humulin 70/30 Pen if there are clumps in the insulin after mixing. Do not use the
84 Humulin 70/30 Pen if solid white particles stick to the walls of the cartridge, giving it a frosted
appearance.

85 Always check the appearance of the Humulin 70/30 suspension in the insulin Pen before using,
86 and if you note anything unusual in the appearance of Humulin 70/30 suspension or notice your
87 insulin requirements changing markedly, consult your doctor.

88 Never attempt to remove the cartridge from the Humulin 70/30 Pen. Inspect the cartridge through
89 the clear cartridge holder.

90 **Storage**

91 **Not in-use (unopened):** Humulin 70/30 Pens not in-use should be stored in a refrigerator but not
92 in the freezer. Do not use a Humulin 70/30 Pen if it has been frozen.

93 **In-use:** Humulin 70/30 Pens in-use should **NOT** be refrigerated but should be kept at room
94 temperature (below 86°F [30°C]) away from direct heat and light. Humulin 70/30 Pens in-use must
95 be discarded **after 10 days**, even if they still contain Humulin 70/30.

96 Do not use Humulin 70/30 Pens after the expiration date stamped on the label.

97 **INSTRUCTIONS FOR INSULIN PEN USE**

98 **It is important to read, understand, and follow the instructions in the “Disposable Insulin**
99 **Delivery Device User Manual” before using. Failure to follow instructions may result in**
100 **getting too much or too little insulin. The needle must be changed and the Pen must be**
101 **primed before each injection to make sure the Pen is ready to dose. Performing these steps**
102 **before each injection is important to confirm that insulin comes out when you push the**
103 **injection button, and to remove air that may collect in the insulin cartridge during normal use.**

104 **Every time you inject:**

- 105 • Use a new needle.
- 106 • Prime to make sure the Pen is ready to dose.
- 107 • Make sure you got your full dose.

108 **NEVER SHARE INSULIN PENS, CARTRIDGES, OR NEEDLES.**

109 **PREPARING THE INSULIN PEN FOR INJECTION**

- 110 1. Always check the appearance of the Humulin 70/30 suspension in the insulin Pen before
111 using.
- 112 2. Roll the Humulin 70/30 Pen between the palms 10 times (*see* Figure 1).
- 113 3. Holding the Humulin 70/30 Pen by one end, invert it 180° slowly 10 times to allow the
114 small glass bead to travel the full length of the cartridge with each inversion (*see* Figure 2).
115 The cartridge is contained in the clear cartridge holder of the Humulin 70/30 Pen.
- 116 4. Inspect the appearance of the Humulin 70/30 suspension to make sure the contents look
117 uniformly cloudy or milky. If not, repeat the above steps until the contents are mixed. Do not
118 use a Humulin 70/30 Pen if there are clumps in the insulin or if solid white particles stick to
119 the walls of the cartridge.
- 120 5. Follow the instructions in the “Disposable Insulin Delivery Device User Manual” for these
121 steps:
 - 122 • Preparing the Pen
 - 123 • Attaching the Needle. **Use a new needle for each injection.**
 - 124 • Priming the Pen. **The Pen must be primed before each injection to make sure the Pen**
125 **is ready to dose.** Performing the priming step is important to confirm that insulin comes
126 out when you push the injection button, and to remove air that may collect in the insulin
127 cartridge during normal use.
 - 128 • Setting a Dose
 - 129 • Injecting a Dose. **To make sure you have received your full dose, you must push the**
130 **injection button all the way down until you see a diamond (◊) or an arrow (®) in the**
131 **center of the dose window.**
 - 132 • Following an Injection

133 **PREPARING FOR INJECTION**

- 134 1. Wash your hands.

- 135 2. To avoid tissue damage, choose a site for each injection that is at least 1/2 inch from the
136 previous injection site. The usual sites of injection are abdomen, thighs, and arms.
- 137 3. Cleanse the skin with alcohol where the injection is to be made.
- 138 4. With one hand, stabilize the skin by spreading it or pinching up a large area.
- 139 5. Inject the dose as instructed by your doctor. Hold the needle under the skin for at least
140 5 seconds after injecting.
- 141 6. After injecting a dose, pull the needle out and apply gentle pressure over the injection site
142 for several seconds. **Do not rub the area.**
- 143 7. Immediately after an injection, remove the needle from the Humulin 70/30 Pen. Doing so
144 will guard against contamination, leakage, reentry of air, and needle clogs. **Do not reuse**
145 **needles.** Place the used needle in a puncture-resistant disposable container and properly
146 dispose of it as directed by your Health Care Professional.

147 **DOSAGE**

148 Your doctor has told you which insulin to use, how much, and when and how often to inject it.
149 Because each patient's case of diabetes is different, this schedule has been individualized for you.

150 Your usual Humulin 70/30 dose may be affected by changes in your food, activity, or work
151 schedule. Carefully follow your doctor's instructions to allow for these changes. Other things that
152 may affect your Humulin 70/30 dose are:

153 **Illness**

154 Illness, especially with nausea and vomiting, may cause your insulin requirements to change.
155 Even if you are not eating, you will still require insulin. You and your doctor should establish a
156 sick day plan for you to use in case of illness. When you are sick, test your blood glucose/urine
157 glucose and ketones frequently and call your doctor as instructed.

158 **Pregnancy**

159 Good control of diabetes is especially important for you and your unborn baby. Pregnancy may
160 make managing your diabetes more difficult. If you are planning to have a baby, are pregnant, or
161 are nursing a baby, consult your doctor.

162 **Medication**

163 Insulin requirements may be increased if you are taking other drugs with hyperglycemic activity,
164 such as oral contraceptives, corticosteroids, or thyroid replacement therapy. Insulin requirements
165 may be reduced in the presence of drugs with blood-glucose-lowering activity, such as oral
166 antidiabetic agents, salicylates (for example, aspirin), sulfa antibiotics, alcohol, and certain
167 antidepressants. Always discuss any medications you are taking with your doctor.

168 **Exercise**

169 Exercise may lower your body's need for insulin during and for some time after the physical
170 activity. Exercise may also speed up the effect of a Humulin 70/30 dose, especially if the exercise
171 involves the area of injection site (for example, the leg should not be used for injection just prior
172 to running). Discuss with your doctor how you should adjust your regimen to accommodate
173 exercise.

174 **Travel**

175 Persons traveling across more than 2 time zones should consult their doctor concerning
176 adjustments in their insulin schedule.

177 **COMMON PROBLEMS OF DIABETES**

178 **Hypoglycemia (Low Blood Sugar)**

179 Hypoglycemia (too little glucose in the blood) is one of the most frequent adverse events
180 experienced by insulin users. It can be brought about by:

- 181 1. Taking too much insulin.
- 182 2. Missing or delaying meals.
- 183 3. Exercising or working more than usual.
- 184 4. An infection or illness (especially with diarrhea or vomiting).

- 185 5. A change in the body's need for insulin.
186 6. Diseases of the adrenal, pituitary or thyroid gland, or progression of kidney or liver
187 disease.
188 7. Interactions with other drugs that lower blood glucose, such as oral antidiabetic agents,
189 salicylates (for example, aspirin), sulfa antibiotics, and certain antidepressants.
190 8. Consumption of alcoholic beverages.

191 Symptoms of mild to moderate hypoglycemia may occur suddenly and can include:

- | | |
|--|-----------------------|
| 192 • sweating | • drowsiness |
| 193 • dizziness | • sleep disturbances |
| 194 • palpitation | • anxiety |
| 195 • tremor | • blurred vision |
| 196 • hunger | • slurred speech |
| 197 • restlessness | • depressed mood |
| 198 • tingling in the hands, feet, lips, or tongue | • irritability |
| 199 • lightheadedness | • abnormal behavior |
| 200 • inability to concentrate | • unsteady movement |
| 201 • headache | • personality changes |

202 Signs of severe hypoglycemia can include:

- | | |
|-----------------------|------------|
| 203 • disorientation | • seizures |
| 204 • unconsciousness | • death |

205 Therefore, it is important that assistance be obtained immediately.

206 Early warning symptoms of hypoglycemia may be different or less pronounced under certain
207 conditions, such as long duration of diabetes, diabetic nerve disease, medications such as beta-
208 blockers, change in insulin preparations, or intensified control (3 or more insulin injections per
209 day) of diabetes.

210 **A few patients who have experienced hypoglycemic reactions after transfer from animal-**
211 **source insulin to human insulin have reported that the early warning symptoms of**
212 **hypoglycemia were less pronounced or different from those experienced with their previous**
213 **insulin.**

214 Without recognition of early warning symptoms, you may not be able to take steps to avoid more
215 serious hypoglycemia. Be alert for all of the various types of symptoms that may indicate
216 hypoglycemia. Patients who experience hypoglycemia without early warning symptoms should
217 monitor their blood glucose frequently, especially prior to activities such as driving. If the blood
218 glucose is below your normal fasting glucose, you should consider eating or drinking sugar-
219 containing foods to treat your hypoglycemia.

220 Mild to moderate hypoglycemia may be treated by eating foods or drinks that contain sugar.
221 Patients should always carry a quick source of sugar, such as candy mints or glucose tablets. More
222 severe hypoglycemia may require the assistance of another person. Patients who are unable to take
223 sugar orally or who are unconscious require an injection of glucagon or should be treated with
224 intravenous administration of glucose at a medical facility.

225 You should learn to recognize your own symptoms of hypoglycemia. If you are uncertain about
226 these symptoms, you should monitor your blood glucose frequently to help you learn to recognize
227 the symptoms that you experience with hypoglycemia.

228 If you have frequent episodes of hypoglycemia or experience difficulty in recognizing the
229 symptoms, you should consult your doctor to discuss possible changes in therapy, meal plans,
230 and/or exercise programs to help you avoid hypoglycemia.

231 **Hyperglycemia and Diabetic Ketoacidosis (DKA)**

232 Hyperglycemia (too much glucose in the blood) may develop if your body has too little insulin.
233 Hyperglycemia can be brought about by:

- 234 1. Omitting your insulin or taking less than the doctor has prescribed.

- 235 2. Eating significantly more than your meal plan suggests.
236 3. Developing a fever, infection, or other significant stressful situation.

237 In patients with type 1 or insulin-dependent diabetes, prolonged hyperglycemia can result in
238 DKA. The first symptoms of DKA usually come on gradually, over a period of hours or days, and
239 include a drowsy feeling, flushed face, thirst, loss of appetite, and fruity odor on the breath. With
240 DKA, urine tests show large amounts of glucose and ketones. Heavy breathing and a rapid pulse
241 are more severe symptoms. If uncorrected, prolonged hyperglycemia or DKA can lead to nausea,
242 vomiting, stomach pains, dehydration, loss of consciousness, or death. Therefore, it is important
243 that you obtain medical assistance immediately.

244 **Lipodystrophy**

245 Rarely, administration of insulin subcutaneously can result in lipoatrophy (depression in the
246 skin) or lipohypertrophy (enlargement or thickening of tissue). If you notice either of these
247 conditions, consult your doctor. A change in your injection technique may help alleviate the
248 problem.

249 **Allergy to Insulin**

250 *Local Allergy* — Patients occasionally experience redness, swelling, and itching at the site of
251 injection of insulin. This condition, called local allergy, usually clears up in a few days to a few
252 weeks. In some instances, this condition may be related to factors other than insulin, such as
253 irritants in the skin cleansing agent or poor injection technique. If you have local reactions, contact
254 your doctor.

255 *Systemic Allergy* — Less common, but potentially more serious, is generalized allergy to
256 insulin, which may cause rash over the whole body, shortness of breath, wheezing, reduction in
257 blood pressure, fast pulse, or sweating. Severe cases of generalized allergy may be life
258 threatening. If you think you are having a generalized allergic reaction to insulin, notify a doctor
259 immediately.

260 **ADDITIONAL INFORMATION**

261 Additional information about diabetes may be obtained from your diabetes educator.

262 **DIABETES FORECAST** is a magazine designed especially for people with diabetes and their
263 families. It is available by subscription from the American Diabetes Association (ADA), P.O. Box
264 363, Mt. Morris, IL 61054-0363, 1-800-DIABETES (1-800-342-2383).

265 Another publication, **COUNTDOWN**, is available from the Juvenile Diabetes Research
266 Foundation International (JDRFI), 120 Wall Street 19th Floor, New York, NY 10005,
267 1-800-533-CURE (1-800-533-2873).

268 Additional information about Humulin and Humulin 70/30 Pens can be obtained by calling The
269 Lilly Answers Center at 1-800-LillyRx (1-800-545-5979).

270 Literature revised XX 2004

271 **Eli Lilly and Company, Indianapolis, IN 46285, USA**

272
273 2.0 PV 3672 AMP PRINTED IN USA

274
275 Copyright © 1998, 2004, Eli Lilly and Company. All rights reserved.

1 3.0 PV 3734 AMP
2

3 **Lilly**

4
5 *Disposable Insulin Delivery Device*

6 **User Manual**
7

8
9 **Instructions for Use**

10 **Read and follow all of these instructions carefully. If you do not follow these instructions**
11 **completely, you may get too much or too little insulin.**

12
13 **Every time you inject:**

- 14 • Use a new needle
- 15 • Prime to make sure the Pen is ready to dose
- 16 • Make sure you got your full dose (see page 18)

17
18 **Also, read the “INFORMATION FOR THE PATIENT” insert**
19 **enclosed in your Pen box.**

20
21 **Pen Features**

- 22 • A multiple dose, disposable insulin delivery device
- 23 (“insulin Pen”) containing 3 mL (300 units) of U-100
- 24 insulin
- 25 • Delivers up to 60 units per dose
- 26 • Doses can be dialed by single units

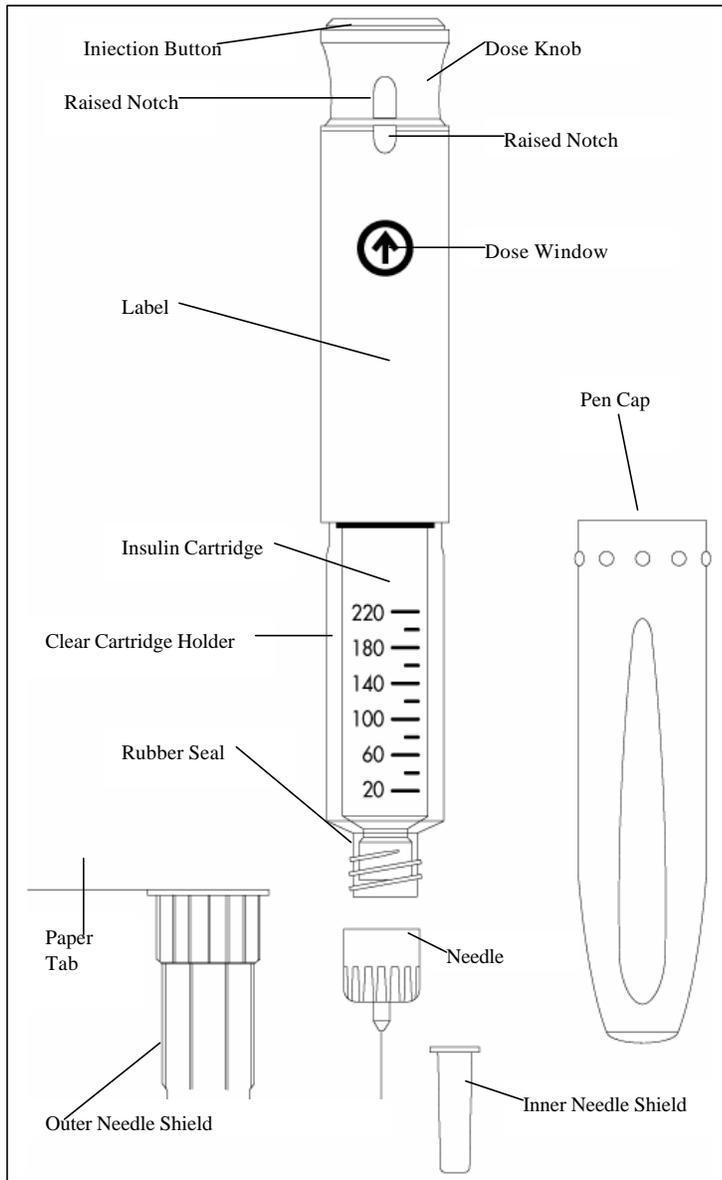


Table of Contents

32	
33	
34	<hr/>
35	Pen Parts3
36	
37	Important Notes 4
38	
39	Preparing the Pen 6
40	
41	Attaching the Needle 8
42	
43	Priming the Pen 10
44	
45	Setting a Dose 14
46	
47	Injecting a Dose 16
48	
49	Following an Injection18
50	
51	Questions and Answers 20
52	<hr/>
53	
54	2

55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93

Pen Parts



94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126

Important Notes

- **Read and follow all of these instructions carefully. If you do not follow these instructions completely, you may get too much or too little insulin.**
- **Use a new needle for each injection.**
- **Be sure a needle is completely attached to the Pen before priming, setting the dose and injecting your insulin.**
- **Prime every time.**
- **The Pen must be primed before each injection to make sure the Pen is ready to dose.** Performing the priming step is important to confirm that insulin comes out when you push the injection button, and to remove air that may collect in the insulin cartridge during normal use. **See Section III. “Priming the Pen”, pages 10-13.**
- **If you do not prime, you may get too much or too little insulin.**
- **Make sure you get your full dose.**
- To make sure you get your full dose, you must push the injection button all the way down until you see a diamond (◆) or an arrow (→) in the center of the dose window. See “Following an Injection”, page 18.
- The numbers on the clear cartridge holder give an estimate of the amount of insulin remaining in the cartridge. Do not use these numbers for measuring an insulin dose.
- Do not share your Pen.

**Important Notes
(Continued)**

127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162

- Keep your Pen out of the reach of children.
- Pens that have not been used (unopened) should be stored in a refrigerator but not in a freezer. Do not use a Pen if it has been frozen. Refer to the “INFORMATION FOR THE PATIENT” insert for complete storage instructions.
- After a Pen is used for the first time, it should **NOT** be refrigerated but should be kept at room temperature [below 86°F (30°C)] and away from direct heat and light.
- An unrefrigerated Pen should be discarded according to the time specified in the “INFORMATION FOR THE PATIENT” insert, even if it still contains insulin.
- Never use a Pen after the expiration date stamped on the label.
- Do not store your Pen with the needle attached. Doing so may allow insulin to leak from the Pen and air bubbles to form in the cartridge. Additionally, with suspension (cloudy) insulins, crystals may clog the needle.
- Always carry an extra Pen in case yours is lost or damaged.
- Dispose of empty Pens as instructed by your Health Care Professional and without the needle attached.
- This Pen is not recommended for use by blind or visually impaired patients without the assistance of a person trained in the proper use of the product.
- The directions regarding needle handling are not intended to replace local, Health Care Professional, or institutional policies.
- **Any changes in insulin should be made cautiously and only under medical supervision.**

163


I. Preparing the Pen

164

1. Before proceeding, refer to the "INFORMATION FOR THE PATIENT" insert for instructions on checking the appearance of your insulin.
2. Check the label on the Pen to be sure the Pen contains the type of insulin that has been prescribed for you.
3. Always wash your hands before preparing your Pen for use.

165

4. Pull the Pen cap to remove.

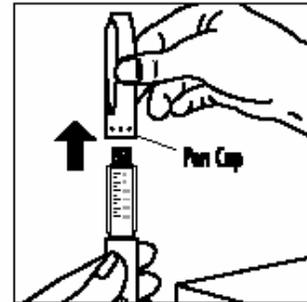


166

167

168
169
170

I. Preparing the Pen (Continued)


5. If your insulin is a suspension (cloudy):
- a. Roll the Pen back and forth 10 times then perform step b.

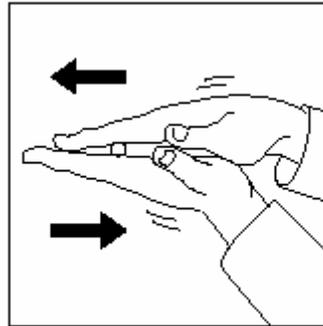

171


- b. Gently turn the Pen up and down 10 times until the insulin is evenly mixed.

Note: Suspension (cloudy) insulin cartridges contain a small glass bead to assist in mixing.

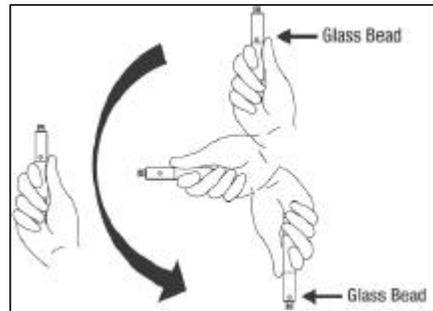

172
173

6. Use an alcohol swab to wipe the rubber seal on the end of the Pen.

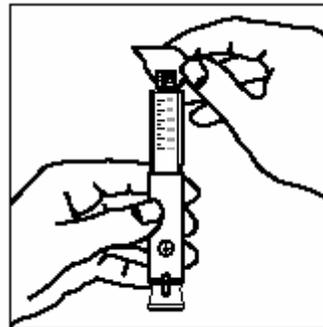

174
175

II. Attaching the Needle


176
177
178
179
180

This device is suitable for use with Becton Dickinson and Company's insulin pen needles.

1. Always use a new needle for each injection. Do not push injection button without a needle attached. Storing the Pen with the needle attached may allow insulin to leak from the Pen and air bubbles to form in the cartridge.


181

2. Remove the paper tab from the outer needle shield.

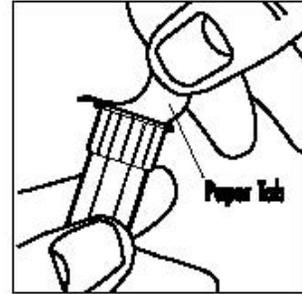

182

3. Attach the capped needle onto the end of the Pen by turning it clockwise until tight.




183
184

185
186
187

II. Attaching the Needle (Continued)

4. Hold the Pen with the needle pointing up and remove the **outer needle shield**. **Keep it to use during needle removal.**

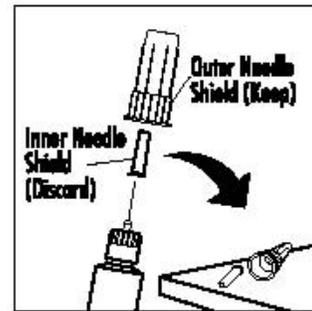

188
189
190
191


5. **Remove the inner needle shield and discard.**

III. Priming the Pen

192
193
194
195
196
197
198
199
200
201


- **The Pen must be primed before each injection to make sure the Pen is ready to dose.**
Performing the priming step is important to confirm that insulin comes out when you push the injection button, and to remove air that may collect in the insulin cartridge during normal use.
- **If you do not prime, you may get too much or too little insulin.**
- **Always use a new needle for each injection.**

1. Make sure the arrow is in the center of the dose window as shown.

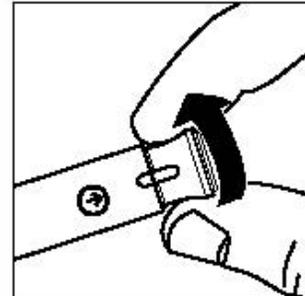

202
203
204
205
206
207
208
209
210
211
212

2. If you do not see the arrow in the center of the dose window, push in the injection button fully and turn the dose knob until the arrow is seen in the center of the dose window.

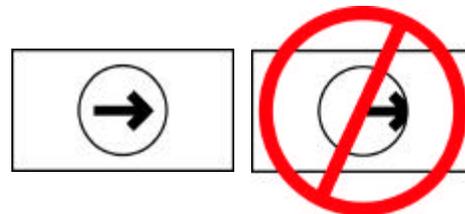


Correct

213
214
215


III. Priming the Pen (Continued)

3. With the arrow in the center of the dose window, pull the dose knob out in the direction of the arrow until a "0" is seen in the dose window.

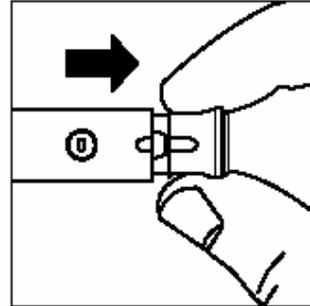

216

4. Turn the dose knob clockwise until the number "2" is seen in the dose window. If the number you have dialed is too high, simply turn the dose knob backward until the number "2" is seen in the dose window.

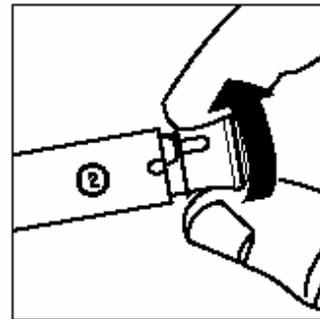

217
218


219
220
221
222

III. Priming the Pen (Continued)

5. Hold your Pen with the needle pointing up. Tap the clear cartridge holder gently with your finger so any air bubbles collect near the top.

Using your thumb, if possible, push in the injection button completely. Keep pressing and continue to hold the injection button **firmly** while counting **slowly** to 5. You should see either a drop or a stream of insulin come out of the tip of the needle.

If insulin does not come out of the tip of the needle, repeat steps 1 through 5. If after several attempts insulin does not come out of the tip of the needle, change the needle and repeat the priming steps.

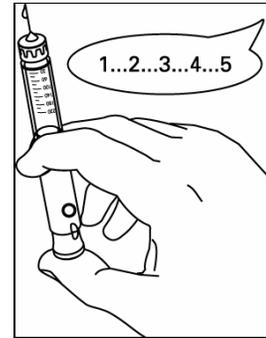

223
224
225


226
227
228

III. Priming the Pen (Continued)

6. At the completion of the priming step, a diamond (◆) must be seen in the center of the dose window. If a diamond (◆) is not seen in the center of the dose window, continue pushing on the injection button until you see a diamond (◆) in the center of the dose window.



229
230
231
232
233
234
235

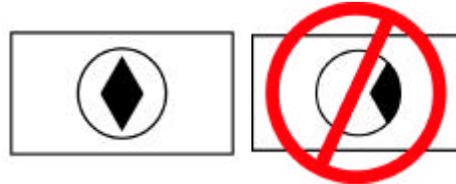

Correct

Note: A small air bubble may remain in the cartridge after the completion of the priming step. If you have properly primed the Pen, this small air bubble will not affect your insulin dose.

7. Now you are ready to set your dose. See next page.

236
237


238
239
240
241
242
243
244
245
246
247
248

IV. Setting a Dose

- **Always use a new needle for each injection. Storing the Pen with the needle attached may allow insulin to leak from the Pen and air bubbles to form in the cartridge.**
- **Caution: Do not push in the injection button while setting your dose. Failure to follow these instructions carefully may result in getting too much or too little insulin. If you accidentally push the injection button while setting your dose, you must prime the Pen again before injecting your dose. See Section III. “Priming the Pen”, pages 10-13.**


1. A diamond must be seen in the center of the dose window before setting your dose.

If you do not see a diamond in the center of the dose window, the Pen has not been primed correctly and you are not ready to set your dose. Before continuing, repeat the priming steps.

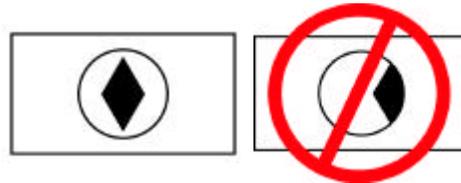

Correct

2. Turn the dose knob clockwise until the arrow (→) is seen in the center of the dose window and the notches on the Pen and dose knob are in line.

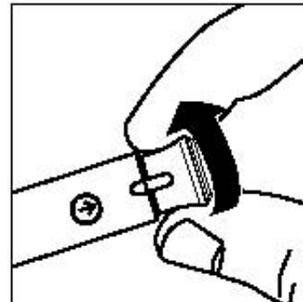

249
250
251


252

IV. Setting a Dose (Continued)

253


254

3. With the arrow (→) in the center of the dose window, pull the dose knob out in the direction of the arrow until a "0" is seen in the dose window. A dose cannot be dialed until the dose knob is pulled out.

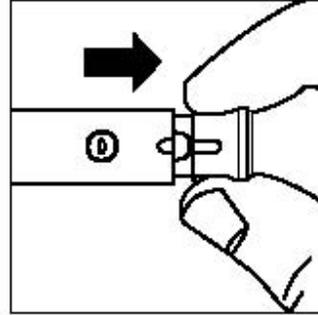

255

4. Turn the dose knob clockwise until your dose is seen in the dose window. If the dose you have dialed is too high, simply turn the dose knob backward until the correct dose is seen in the dose window.

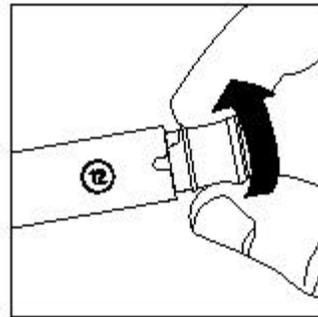

256

5. If you cannot dial your full dose, see the "Questions and Answers" section, Question 5, at the end of this manual.

257

V. Injecting a Dose


258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277

- **Always use a new needle for each injection. Storing the Pen with the needle attached may allow insulin to leak from the Pen and air bubbles to form in the cartridge.**
- **Caution: Do not attempt to change the dose after you begin to push in the injection button. Failure to follow these instructions carefully may result in getting too much or too little insulin.**
- **The effort needed to push in the injection button may increase while you are injecting your insulin dose. If you cannot completely push in the injection button, refer to the “Questions and Answers” section, Question 7, at the end of this manual.**
- **Do not inject a dose unless the Pen is primed, just before injection, or you may get too much or too little insulin.**
- **If you have set a dose and pushed in the injection button without a needle attached or if no insulin comes out of the needle, see the “Questions and Answers” section, Questions 1 and 2.**

278
279
280

V. Injecting a Dose (Continued)


1. Wash hands. Prepare the skin and use the injection technique recommended by your Health Care Professional.
2. Insert the needle into your skin. Inject the insulin by using your thumb, if possible, to push in the injection button completely.



281
282

3. Keep pressing and continue to hold the injection button **firmly** while counting **slowly** to 5.

After counting to 5, pull the needle out and apply gentle pressure over the injection site for several seconds. **Do not rub the area.**

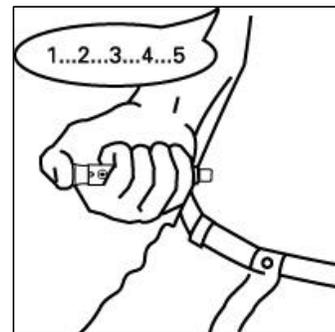

283
284

4. When the injection is done, a diamond (◆) or arrow (→) must be seen in the center of the dose window. This means your full dose has been delivered. **If you do not see the diamond or arrow in the center of the dose window, you did not get your full dose. Contact your Health**




Correct




for additional

285
286
287
288
289
290
291
292
293
294
295
296
297
298



Correct



299
300
301


VI. Following an Injection

1. Make sure you got your full dose by checking that the injection button has been completely pushed in and you can see a diamond (◆) or arrow (→) in the center of the dose window. If you do not see the diamond (◆) or arrow (→) in the center of the dose window, you have not received your full dose. Contact your Health Care Professional for additional instructions.



302

2. Carefully replace the **outer needle shield** as instructed by your Health Care Professional.

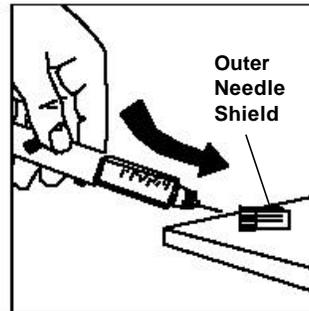


303
304
305
306
307

308
309
310


VI. Following an Injection (Continued)

3. Remove the capped needle by turning it counterclockwise. Place the used needle in a puncture-resistant disposable container and properly throw it away as directed by your Health Care Professional.

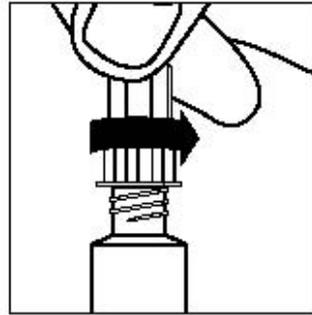

311

4. Replace the cap on the Pen.

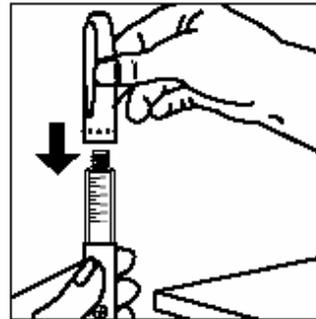

312
313
314
315
316
317
318
319
320
321
322

5. The Pen that you are using should **NOT** be refrigerated but should be kept at room temperature below 86°F (30°C) and away from direct heat and light. It should be discarded according to the time specified in the “INFORMATION FOR THE PATIENT” insert, even if it still contains insulin.

Do not store or dispose of the Pen with a needle attached. Storing the Pen with the needle attached may allow insulin to leak from the Pen and air bubbles to form in the cartridge.

323

324

325

Questions and Answers

Problem	Action
1. Dose dialed and injection button pushed in without a needle attached.	To obtain an accurate dose you must: 1) Attach a new needle. 2) Push in the injection button completely (even if a “0” is seen in the window) until a diamond (◆) or arrow (→) is seen in the center of the dose window. 3) Prime the Pen.
2. Insulin does not come out of the needle.	To obtain an accurate dose you must: 1) Attach a new needle. 2) Push in the injection button completely (even if a “0” is seen in the window) until a diamond (◆) or arrow (→) is seen in the center of the dose window. 3) Prime the Pen. See Section III. “Priming the Pen”, pages 10-13.

326

327

328
329
330

Questions and Answers (Continued)

Problem	Action
3. Wrong dose (too high or too low) dialed.	If you have not pushed in the injection button, simply turn the dose knob backward or forward to correct the dose.
4. Not sure how much insulin remains in the cartridge.	Hold the Pen with the needle end pointing down. The scale (20 units between marks) on the clear cartridge holder shows an estimate of the number of units remaining. These numbers should not be used for measuring an insulin dose.

331
332
333

334
335
336**Questions and Answers
(Continued)**

Problem	Action
5. Full dose cannot be dialed.	The Pen will not allow you to dial a dose greater than the number of insulin units remaining in the cartridge. For example, if you need 31 units and only 25 units remain in the Pen, you will not be able to dial past 25. Do not attempt to dial past this point. (The insulin that remains is unusable and not part of the 300 units.) If a partial dose remains in the Pen you may either: 1) Give the partial dose and then give the remaining dose using a new Pen, or 2) Give the full dose with a new Pen.
6. A small amount of insulin remains in the cartridge but a dose cannot be dialed.	The Pen design prevents the cartridge from being completely emptied. The Pen has delivered 300 units of usable insulin.

337
338
339

340
341
342**Questions and Answers
(Continued)**

Problem	Action
7. Cannot completely push in the injection button when priming the Pen or injecting a dose.	<ol style="list-style-type: none">1) Needle is not attached or is clogged.<ol style="list-style-type: none">a. Attach a new needle.b. Push in the injection button completely (even if a "0" is seen in the window) until a diamond (◆) or arrow (→) is seen in the center of the dose window.c. Prime the Pen.2) If you are sure insulin is coming out of the needle, push in the injection button more slowly to reduce the effort needed and maintain a constant pressure until the injection button is completely pushed in.

343
344

**For additional information call,
1-800-LillyRx (1-800-545-5979)**

Literature revised XX 2004

Eli Lilly and Company, Indianapolis, IN 46285, USA

3.0 PV 3734 AMP

PRINTED IN USA

Lilly

3 mL

Lilly

5 x 3 mL disposable insulin delivery devices
100 Units per mL

Humulin® 70/30 Pen

70% human insulin isophane suspension
30% human insulin injection
(rDNA origin)

disposable insulin delivery device
For information call 1-800-545-5979

HP 8770



5 x 3 mL disposable insulin delivery devices

NDC 0002-8770-59
HP 8770
100 Units per mL

Humulin® 70/30 Pen

70% human insulin isophane suspension
30% human insulin injection
(rDNA origin)

disposable insulin delivery device

Important
Please read updated User Manual
Every time you inject:
/ Use a new needle
/ Prime to make sure the Pen is ready to dose
/ Make sure you got your full dose



This device is suitable for use with Becton Dickinson and Company's insulin pen needles (needles not included)

3 mL

Lilly

5 x 3 mL disposable insulin delivery devices
100 Units per mL

Humulin® 70/30 Pen

70% human insulin isophane suspension
30% human insulin injection
(rDNA origin)

disposable insulin delivery device

HP 8770




A1.0 NL 2483 AMS

A1.0 NL 2483 AMS
A1.0 NL 2483 AMS



Exp. Date / Control No.



If the seal is broken before first use, contact pharmacist



3 0002-8770-59 7

IMPORTANT-SEE WARNINGS ON ENCLOSED INSERT

Lilly

Eli Lilly and Company
Indianapolis, IN 46285, USA
1-800-545-5979

**Shake Carefully Before Using,
See Enclosed Insert for Proper Technique.**

For subcutaneous use.
As with any drug, if you are pregnant or nursing a baby, seek professional advice when using this product.

Keep in a cold place. Avoid freezing.
Warning: Any change of insulin should be made cautiously and only under medical supervision. See enclosed insert.

If the seal is broken before first use, contact pharmacist

C-1004

disposable insulin delivery device



3 mL *Lilly*
Humulin® 70/30 Pen
70% human insulin isophane suspension
30% human insulin injection
(rDNA origin)

5 x 3 mL disposable insulin delivery devices
100 Units per mL

HP 8770