

12 9 74720  
510(k) Summary

MAR 13 1998

Proprietary Name: Howmedica® Fully Threaded Screws  
Common Name: Intramedullary Rod  
Classification Name & Reference: Intramedullary Fixation Rod  
21 CFR 888.3020  
Proposed Regulatory Class: II  
Device Product Code: 87HSB

For information contact: Vivian Kelly  
Manager, Regulatory Affairs  
Howmedica Inc.  
359 Veterans Boulevard  
Rutherford, NJ 07070  
Telephone: (201) 507-7830  
Fax: (201) 507-6870

Howmedica's Locking Nail Systems consist of different types of intramedullary nails/rods, cross-locking screws and end caps. This line extension is to add a smaller cross-locking screw for use with current Howmedica® IM rod and nail systems cleared under various 510(k) notifications plus any future styles of stainless steel IM rods or nails. The new screw is 3.7mm in diameter and is available in various lengths. It has a cortical buttress thread design for cross-locking of IM nails. The screws are manufactured from medical grade stainless steel.

The Howmedica® Fully Threaded Screws are intended to be used for cross-locking of intramedullary nails and IM rods.

The substantial equivalence of these components is based on an equivalence in intended use, materials, design, and operational principles to Howmedica's 4.6mm Fully Threaded Screws, Zimmer's Buttress Thread Screws and Zimmer's ZMS Recon Nail Cross-Locking Screw.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

Food and Drug Administration  
9200 Corporate Boulevard  
Rockville MD 20850

MAR 13 1998

Ms. Vivian Kelly  
Manager, Regulatory Affairs  
Howmedica, Inc.  
Pfizer Hospital Products Group  
359 Veterans Boulevard  
Rutherford, New Jersey 07070-2584

Re: K974720  
Trade Name: Howmedica® Fully Threaded Screws  
Regulatory Class: II  
Product Code: HSB  
Dated: December 17, 1997  
Received: December 18, 1997

Dear Ms. Kelly:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

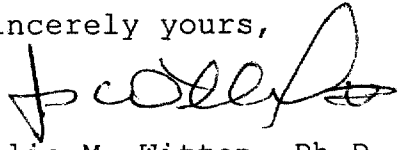
If your device is classified (see above) into either class II (Special Controls) or class III (Premarket Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the current Good Manufacturing Practice requirement, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic (QS) inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

Page 2 - Ms. Vivian Kelly

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4659. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its internet address "<http://www.fda.gov/cdrh/dsmamain.html>".

Sincerely yours,

  
fr Celia M. Witten, Ph.D., M.D.  
Director  
Division of General and  
Restorative Devices  
Office of Device Evaluation  
Center for Devices and  
Radiological Health

Enclosure

**Indications for Use**

510(k) Number (if known): K974720

Device Name: Howmedica® Fully Threaded Screws

Indications for Use:

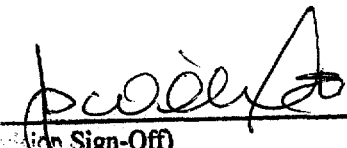
The Howmedica® 3.7mm Fully Threaded Screws are intended to be used for cross-locking of Howmedica's intramedullary nails and IM rods.

(PLEASE DO NOT WRITE BELOW THIS LINE - CONTINUE ON ANOTHER PAGE IF NEEDED)

\_\_\_\_\_  
Concurrence of CDRH, Office of Device Evaluation (ODE)

Prescription Use X OR Over-The-Counter Use \_\_\_\_\_  
(Per 21 CFR 801.109)

(Optional Format 1-2-96)

  
(Signature Sign-Off)  
General Restorative Devices  
510(k) Number K974720