

JUL 13 1998



K982154

Regulatory Affairs Department

**TOWNLEY Pedicle Screw Plating System
510(k) Summary**

**I. Company: Sofamor Danek USA
1800 Pyramid Place
Memphis, TN 38132
(901) 396-3133**

II. Proprietary Trade Name: TOWNLEY Pedicle Screw Plating System

III. Product Description

This system consists of a broad-headed, partially threaded screw designed to compress bone grafts. Screw lengths range from 0.5 to 2.5 inches. Both cortical and cancellous screw threads are available. The screw comes in two configurations: flat-head or hex. The hex screws are slightly wider in diameter. The stainless steel DYNA-LOK® plates are used to interconnect two or more vertebrae together via screw fixation through the pedicles. All components are fabricated from medical grade stainless steel (ASTM F-138 or its ISO equivalent).

IV. Indications

The TOWNLEY Pedicle Screw Plating System is intended to stabilize the spine as an aid to fusion. After first making drill holes in the pedicles, a DYNA-LOK® plate is positioned of the pedicles. TOWNLEY Pedicle screws are then inserted through the DYNA-LOK® plate, down the center of the pedicles, and into the vertebral body. Bone graft must be used with each procedure.

This system is indicated for the treatment of any or all of the following at the C2 to S1 (inclusive) spinal levels: (a) Trauma, including spinal fractures and/or dislocations; (b) Spondylolisthesis; (c) Spondylolysis; (d) Pseudarthrosis or failed previous fusions which are symptomatic or which may cause secondary instability or deformity; (e) Degenerative disc disease and/or degenerative diseases which include: (1) degenerative disc disease (DDD) as defined by neck and/or back pain of discogenic origin as confirmed by radiographic studies; and/or (2) degenerative disease of the facets with instability.

V. Substantial Equivalence

Documentation was provided which demonstrated the TOWNLEY Pedicle Screw Plating System was demonstrated to be substantially equivalent to itself.

000025



JUL 13 1998

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

Richard W. Treharne, Ph.D.
Vice President
Research and Regulatory Affairs
Sofamor Danek
1800 Pyramid Place
Memphis, Tennessee 38132

Re: K982154
Townley Pedicle Screw Plating System
Regulatory Class: II
Product Codes: MNI, MNH and KWP
Dated: June 18, 1998
Received: June 19, 1998

Dear Dr. Treharne:

We have reviewed your Section 510(k) notification of intent to market the device system referenced above and we have determined the device system is substantially equivalent (for the indications for use stated in the enclosure) to device systems marketed in interstate commerce prior to May 28, 1976 or to devices that have been reclassified in accordance with the provisions of the Federal, Food, Drug, and Cosmetic Act (Act).

You may, therefore, market your device system subject to the general controls provisions of the Act and the limitations identified below. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration. Note that labeling or otherwise promoting this device system for pedicular screw fixation/attachment for indications other than that described in item 2 below, would cause the device system to be adulterated under 501(f)(1) of the Act.

This device system, when intended for pedicular screw fixation/attachment to the spine for indications other than that described in item 2 below, is a class III device under Section 513(f) of the Act. Class III devices are required to have an approved premarket approval (PMA) application prior to marketing. Accordingly:

1. The package label must state that there are labeling limitations.
2. The package insert must prominently state that the device system, as a pedicle screw fixation system, is intended only for the following:

- a. trauma, including fractures and/or dislocations;
- b. degenerative disc disease and/or degenerative diseases which include:
 - (1) degenerative disc disease (ddd) as defined by back and/or neck pain of discogenic origin as confirmed by patient history with degeneration of the disc as confirmed by radiographic studies and/or
 - (2) degenerative disease of the facets with instability;
- c. spondylolysis;
- d. spondylolisthesis, all grades and types; and
- e. pseudarthrosis.

For all of these indications, bone graft must be used and the system is limited to screw fixation from C2 to S1; and

3. The package insert must also include the following **WARNINGS**:

- As a pedicle screw fixation system, this subject system is intended only for the following:
 - trauma, including fractures and/or dislocations;
 - degenerative disc disease and/or degenerative diseases which include:
 - (1) degenerative disc disease (ddd) as defined by back and/or neck pain of discogenic origin as confirmed by patient history with degeneration of the disc as confirmed by radiographic studies and/or
 - (2) degenerative disease of the facets with instability;
 - spondylolysis;
 - spondylolisthesis, all grades and types; and
 - pseudarthrosis.

For all of these indications, bone graft must be used and the system is limited to screw fixation from C2 to S1.

- Benefit of spinal fusions utilizing any pedicle screw fixation system has not been adequately established in patients with stable spines.
- Potential risks identified with the use of this device system, which may require additional surgery, include: device component fracture, loss of fixation, non-union, fracture of the vertebra, neurological injury, and vascular or visceral injury.

See Warnings, Precautions, and Potential Adverse Events sections of the package insert for a complete list of potential risks.

4. Any pedicular screw fixation/attachment for intended uses other than that described by item 2 above, for this device is considered investigational and may only be investigated as a significant risk device in accordance with the investigational device exemption (IDE) regulations under 21 CFR, Part 812. All users of the device for pedicular screw fixation/attachment for intended uses other than that described above, must receive approval from their respective institutional review boards (IRBs) and the Food and Drug Administration (FDA) prior to conducting an investigation.
5. Any previous warning statements identified as part of previous 510(k) clearances or required by OC/Labeling and Promotion which stated that a component/system was not approved for screw fixation into the pedicles of the spine must be replaced by the warnings of item 3 above.


FDA advises that the use of your device system with any other device components but those identified in this 510(k) would require submission of a new 510(k) providing documentation of design, material, and labeling compatibility between the device components. Mechanical testing of a spinal system consisting of the subject device components and other device components, whether yours or those of other manufacturers, may also be required.

If your device is classified (see above) into either class II (Special Controls) or class III (Premarket Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the current Good Manufacturing Practice requirement, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic (QS) inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal Laws or Regulations.

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification immediately. An FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4659. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or at (301) 443-6597, or at its Internet address "<http://www.fda.gov/cdrh/dsmamain.html>".

Sincerely yours,

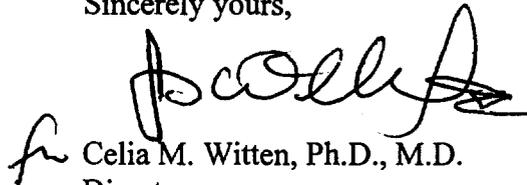A handwritten signature in black ink, appearing to read "Celia M. Witten". The signature is written in a cursive style with a large initial "C".

Celia M. Witten, Ph.D., M.D.
Director
Division of General and
Restorative Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

510(k) Number (if known): K982154

Device Name: TOWNLEY Pedicle Screw Plating System

Indications for Use:


The TOWNLEY Pedicle Screw Plating System is intended to stabilize the spine as an aid to fusion. After first making drill holes in the pedicles, a DYNA-LOK® plate is positioned of the pedicles. TOWNLEY Pedicle screws are then inserted through the DYNA-LOK® plate, down the center of the pedicles, and into the vertebral body. Bone graft must be used with each procedure.

This system is indicated for the treatment of any or all of the following at the C2 to S1 (inclusive) spinal levels: (a) Trauma, including spinal fractures and/or dislocations; (b) Spondylolisthesis; (c) Spondylolysis; (d) Pseudarthrosis or failed previous fusions which are symptomatic or which may cause secondary instability or deformity; (e) Degenerative disc disease and/or degenerative diseases which include: (1) degenerative disc disease (DDD) as defined by neck and/or back pain of discogenic origin as confirmed by radiographic studies; and/or (2) degenerative disease of the facets with instability.

(PLEASE DO NOT WRITE BELOW THIS LINE—CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDRH, Office of Evaluation (ODE)

Prescription Use X OR Over-the-counter Use _____
(Per 21 CFR 801.109)
(Optional 1-2-96)

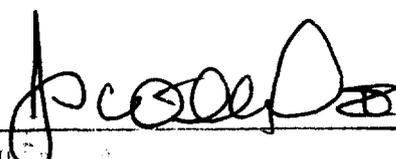

(Division of)
Division of Devices K982154
510(k) Number