

K982602

510(k) Summary

Proprietary Name:	Retrograde Rod System
Common Name:	IM Rod
Classification Name & Reference:	Intramedullary Fixation Rod 21 CFR 888.3020
Regulatory Class:	II
Device Product Code:	87HSB

For information contact: Vivian Kelly
Manager, Regulatory Affairs
Howmedica Inc.
359 Veterans Boulevard
Rutherford, NJ 07070
Telephone: (201) 507-7830
Fax: (201) 507-6870

Date prepared: July 24, 1998

The Alta® IM Rod System consists of a family of curved, fluted rods, cross-locking screws and cap screws for intramedullary nailing of femoral, tibial and humeral fractures. The new Retrograde Rod is intended for stabilizing various types of fractures, osteotomies, malunions, and nonunions of the femur. The rods can be inserted with or without reaming and can be statically or dynamically locked.

This submission is a modification of the currently marketed Alta IM rods and cap screws cleared under various 510(k) notifications. The new femoral IM rods will have proximal and distal holes for dynamic or static locking. There will also be a dynamic slot design for dynamic locking. They will be available in various configurations including round and fluted designs, solid or cannulated rods in diameters ranging from 9mm to 14 mm in various lengths. A new cap screw will be available with extended ends. These new components will be used with cross-locking screws and other rod components previously cleared under different premarket notifications.

The substantial equivalence of these components is based on an equivalence in intended use, materials, design, and operational principles to Howmedica's Alta® IM Rod System, Synthes' Ti DFN System, and ACE Medical's ART™ Femoral Nail System.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

SEP 14 1998

Ms. Vivian Kelly
Manager, Regulatory Affairs
Howmedica Inc.
Pfizer Hospital Products Group
359 Veterans Boulevard
Rutherford, New Jersey 07070-2584

Re: K982602
Trade Name: ALTA® A-P Rod Modification
Regulatory Class: II
Product Code: HSB
Dated: July 24, 1998
Received: July 27, 1998

Dear Ms. Kelly:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

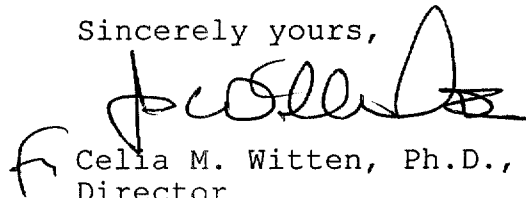
If your device is classified (see above) into either class II (Special Controls) or class III (Premarket Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the current Good Manufacturing Practice requirement, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic (QS) inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

Page 2 - Ms. Vivian Kelly

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4659. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its internet address "<http://www.fda.gov/cdrh/dsmamain.html>".

Sincerely yours,


F Celia M. Witten, Ph.D., M.D.
Director
Division of General and
Restorative Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

Indications for Use

510(k) Number (if known):

Device Name: ALTA® A-P ROD MODIFICATION

Indications for Use:

The Alta® IM Rod System consists of a family of curved, fluted rods, cross-locking screws and cap screws for intramedullary nailing of femoral, tibial and humeral fractures. The new Retrograde Rod is intended for stabilizing various types of fractures, osteotomies, malunions, and nonunions of the femur. The rods can be inserted with or without reaming and can be statically or dynamically locked.

(PLEASE DO NOT WRITE BELOW THIS LINE - CONTINUE ON ANOTHER PAGE IF NEEDED)

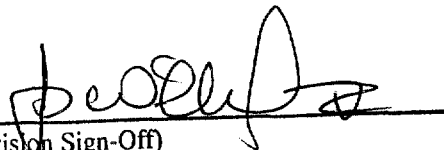
Concurrence of CDRH, Office of Device Evaluation (ODE)

Prescription Use X
(Per 21 CFR 801.109)

OR

Over-The-Counter Use _____

(Optional Format 1-2-96)


(Division Sign-Off)
Division of General Restorative Devices

510(k) Number

K982602