

SEP 22 1999

K992306

510(k) Summary of Safety and Effectiveness

This 510(k) summary of safety and effectiveness information is being submitted in accordance with the requirements of SMDA 1990.

Date Prepared:

June 30, 1999

Submitter's Information: 21 CFR 807.92(a)(1)

SAMSUNG SDS CO., LTD

707-19, Yoksam-Dong, Kangnam-Gu,

Seoul, South Korea, 135-080

Trade Name, Common Name and Classification: 21 CFR 807.92(a)(2)

Trade Name: Samsung RAYPAX™ Display Workstation System

Common Name: Digital Imaging Workstation

Classification Name: System, Digital Image Communication accessory

Device Classification: 21 CFR 892.2020

Predicate Device: 21 CFR 807.92(a)(3)

Manufacturer: Olicon Imaging Systems, Inc

Device: 02-Workstation & PACS View Software

510(k) Number: K973959

Date Received: 10/16/97

Decision Date: 12/22/97

Decision: Substantially Equivalent

Panel Code device reviewed by: Radiology

Panel Code device classified by: Radiology

Product Code: 90 LMD

Classification: Class II

Device Description: 21 CFR 807.92(a)(4)

The Display Workstation is one of the components of the RAYPAX, a PACS solution by Samsung or can be a separate device for other manufacturer's PACS. The Display Workstation provides image-processing functions and workflow for the radiology department for medical images that are acquired and stored in the RAYPAX image server in DICOM 3.0 format.

Furthermore, the Display Workstation can transfer medical images stored in RAYPAX system to other PACS through a DICOM compatible network and can export images to other applications in bitmap format.

Indications for Use: 21 CFR 807 92(a)(5)

The Samsung RAYPAX™ Display Workstation is a device that receives digital images and data from various image sources, (including but not limited to CT Scanners, MR Scanners, Ultrasound Systems, R/F Units, Computed & Direct Radiographic devices, secondary capture devices, film scanners, imaging gateways, or other imaging sources). Images and data can be stored, communicated, processed, and displayed within the workstation or across computer networks at distributed locations.

The typical users of this system are trained professionals, including but not limited to physicians, nurses, and medical technicians.

Technological Characteristics: 21 CFR 807 92(a)(6)

The device does not contact the patient, nor does it control any life sustaining devices. A physician, providing ample opportunity for competent human intervention interprets images and information being printed.

Conclusion: 21 CFR 807 92(b)(1)

The 510(k) Pre-Market Notification for the Samsung Display Workstation contains adequate information and data to enable FDA - CDRH to determine substantial equivalence to the predicate device.

1. The RAYPAX™ Display Workstation system has been and will be manufactured in accordance with the voluntary standards listed in the enclosed voluntary standard survey.
2. The submission contains the results of a hazard analysis and all potential hazards have been classified as Minor.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

SEP 22 1999

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

Samsung SDS Co., LTD.
C/O Mr. Carl Aletto
OTECH, Inc.
2001 East Oakshores Drive
Aubrey, TX 76227

Re: K992306
Samsung RAYPAX™ Display Workstation
Dated: June 30, 1999
Received: July 9, 1999
Regulatory Class: II (TWO)
Product Code: 90 LLZ
21 CFR 892.2050

Dear Mr. Aletto:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

If your device is classified (see above) into either class II (Special Controls) or class III (Premarket Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the Current Good Manufacturing Practice requirements, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic QS inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4613. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597, or at its internet address "<http://www.fda.gov/cdrh/dsma/dsmamain.html>".

Sincerely yours,

CAPT Daniel G. Schultz, M.D.
Acting Director, Division of Reproductive,
Abdominal, Ear, Nose and Throat,
and Radiological Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

R

(Indications for Use Form)

510(k) Number:

Device Name:

Samsung SDS Co. Ltd. RAYPAX™ Display Workstation System

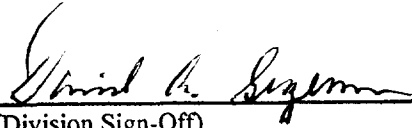
Indications for Use:

The Samsung RAYPAX™ Display Workstation is a device that receives digital images and data from various image sources, (including but not limited to CT Scanners, MR Scanners, Ultrasound Systems, R/F Units, Computed & Direct Radiographic devices, secondary capture devices, film scanners, imaging gateways, or other imaging sources). Images and data can be stored, communicated, processed, and displayed within the workstation or across computer networks at distributed locations.

The typical users of this system are trained professionals, including but not limited to physicians, nurses, and medical technicians.

(PLEASE DO NOT WRITE BELOW THIS LINE - CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDRH, Office of Device Evaluation (ODE)


(Division Sign-Off)
Division of Reproductive, Abdominal, ENT,
and Radiological Devices
510(k) Number K992306

Prescription Use ☒
(Per 21 CFR 801.109)

OR

Over-The-Counter Use ☐

(Optional Format 1-2-96)