

K120470/S001

510(k) Summary for Watermark Medical Mobile Application

Submitter: Watermark Medical
Address: 1750 Clint Moore Road, Suite 101 □
Boca Raton, FL 33487
Corporate Contact: Frank Katarow, Chief Operating Officer
WaterMark Medical
Telephone: 877-710-6999
Establishment Registration #: 3008208119
Submission Contact: Michael J. Leigh, consultant
12715 Falcon Drive
Brookfield, Wisconsin 53005
Ph: (262) 957-6797

JUN - 8 2012

Trade Name: MiPal
Predicate Device: Honeywell HomMed Genesis OTC, K061087
Common Name: Patient Vital Signs Monitor
Classification Name:

Regulation Number	Product Code	Classification Name	Device Class
870.2910	DRG	Transmitters And Receivers, Physiological Signal, Radiofrequency	II
<i>Medical device product codes also supported by MiPal by means of separate medical devices</i>			
870.1130	DXN	Noninvasive Blood Pressure Measurement System	II
880.2700	FRI	Patient Weight Scale	I
870.2700	DQA	Oximeter	II
862.1345	NBW	Glucose Test System	II

Device Description:

The MiPal is a communication hub intended to receive and transmit patient information on a retrospective basis. The device is not intended for real-time monitoring or emergency use by patients or caregivers.

The MiPal is designed to optionally collect NiBP, pulse, and SpO2. It may also collect other vitals through the vitals acquisition process via Bluetooth medical peripherals.

Peripherals will include:

- Scale
- Glucose meter

K120470/S001

Intended Use:

MiPal allows the user to collect vital signs data (including noninvasive blood pressure, pulse rate, weight and other data from optional add-on devices). The user can then transmit the data to a central database via a communication network. Use of the system allows retrospective review of certain physiological functions by qualified health care professionals. The MiPal is intended for use with adult and pediatric patients over twelve years of age.

SpO2 is to be used under the direction of licensed health care professionals, and is available only by or on the order of a physician.

Performance Data:

The verification and validation results demonstrated that the MiPal was in compliance with the guidelines and standards referenced in the FDA reviewer's guides and that it performed within its specifications and functional requirements.

This summary of 510(k) safety and effectiveness information is being submitted in accordance with the requirements of FDA.



Food and Drug Administration
10903 New Hampshire Avenue
Document Control Room -WO66-G609
Silver Spring, MD 20993-0002

JUL 11 2012

Watermark Medical, Inc
c/o Michael J. Leigh
Consultant
12715 Falcon Drive
Brookfield, Wisconsin 53005

Re: K120470/S001
Trade Name: MiPal, Patient Vital Signs Monitor
Regulatory Number: 21 CFR 870.2910
Regulation Name: Radiofrequency physiological signal transmitter and receiver
Regulatory Class: II (two)
Product Code: DRG
Dated: May 22, 2012
Received: May 31, 2012

Dear Mr. Leigh:

This letter corrects our substantially equivalent letter of June 8, 2012.

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and

adulteration. Please note: CDRH does not evaluate information related to contract liability warranties. We remind you, however, that device labeling must be truthful and not misleading.


If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); medical device reporting (reporting of medical device-related adverse events) (21 CFR 803); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please go to <http://www.fda.gov/AboutFDA/CentersOffices/CDRH/CDRHOffices/ucm115809.htm> for the Center for Devices and Radiological Health's (CDRH's) Office of Compliance. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to <http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/default.htm> for the CDRH's Office of Surveillance and Biometrics/Division of Postmarket Surveillance.

You may obtain other general information on your responsibilities under the Act from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 796-7100 or at its Internet address <http://www.fda.gov/MedicalDevices/ResourcesforYou/Industry/default.htm>.

Sincerely yours,

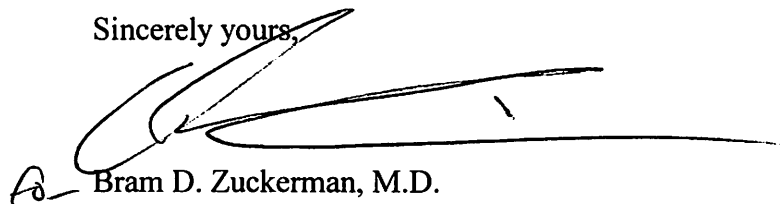

Bram D. Zuckerman, M.D.
Director
Division of Cardiovascular Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

Indications for Use

510(k) Number (if known): K120470/S001

Device Name: Watermark Medical MiPal

Indications For Use:

MiPal allows the user to collect vital signs data (including noninvasive blood pressure, pulse rate, weight and other data from optional add-on devices). The user can then transmit the data to a central database via a communication network. Use of the system allows retrospective review of certain physiological functions by qualified health care professionals. It is not intended for real-time, emergency, or critical care monitoring of patient vital signs. The MiPal is intended for use with adult and pediatric patients over twelve years of age.

SpO2 is to be used under the direction of licensed health care professionals, and is available only by or on the order of a physician.

Prescription Use
 (Part 21 CFR 801 Subpart D)

AND/OR

Over-The-Counter Use
 (21 CFR 807 Subpart C)

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDRH, Office of Device Evaluation (ODE)


(Division Sign-Off)
Division of Cardiovascular Devices

510(k) Number K120470