

**510(K) SUMMARY**

This summary of 510(k) safety and effectiveness information is being submitted in accordance with the requirements of SMDA 1990 and 21 CFR 807.92.

The assigned 510(k) number is: K021359

1. Submitter's Identifications:

Well-Life Healthcare Inc.  
Room 6C01, No. 5, Sec. 5, Hsin Yi Rd.,  
Taipei, Taiwan, R.O.C.

Contact:  
Ms. Grace Chang  
Sales Manager

Date of Summary Preparation: December, 2001.

2. Name of the Device:

Well-Life TENS (Transcutaneous Electrical Nerve Stimulation Device), Model Digi-Pro TENS series, including WL-2203, WL-2204, and WL-2205.

3. Information of the 510(k) Cleared Device (Predicate Device):

Please see the information provided in part 6 of this summary.

4. Device Description:

The Digi-Pro TENS series, including WL-2203, WL-2204, and WL-2205 are transcutaneous electrical nerve stimulator used for pain relief and/or powered muscle stimulator by applying an electrical current to electrodes, which are attached on the patient's skin. The output and waveform is adjustable according to the situation of patient.

Digi-Pro TENS series, models WL-2203, WL-2204, and WL-2205, consist mainly of two parts: the stimulus generator, electrode. The stimulus generator generates the output current specified as the input of controller. The output port transmits the output current to the electrode, which is attached to the patient's skin so as to transmit this stimulus current to the patient for pain relief.

The stimulation mode for Digi-Pro TENS includes several different operation modes as mentioned on the comparison table. These operation modes are generated from the software control by using the microprocessor as its main control unit.

5. Intended Use:

On the instruction manual of each model, the intended uses and contraindication are defined very clearly. Please see the information of instruction manuals in clause 7.6 of this submission document.

In addition, the standard format for the statement of indications and contraindication for use are provided hereafter.



Food and Drug Administration  
9200 Corporate Boulevard  
Rockville MD 20850

Mr. Tony C.S. Chang  
Well-Life Healthcare Inc.  
C/o Wincent Consultant  
No. 5, Alley 5, Lane Cheng Hsing  
Chung Ching Road, Pei Tun Dist.  
Taichung, Taiwan, R.O.C.

APR 30 2002

Re: K021359

Trade/Device Name: Digi-Pro TENS models WL-2203 and WL-2205  
Regulation Number: 21 CFR 882.5890  
Regulation Name: Transcutaneous electrical nerve stimulator for pain relief  
Regulatory Class: Class II  
Product Code: GZJ  
Dated: January 18, 2002  
Received: January 30, 2002

Dear Mr. Tony Chang:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.


If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic

product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050. This letter will allow you to begin marketing your device as described in your Section 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 21 CFR Part 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its Internet address <http://www.fda.gov/cdrh/dsma/dsmamain.html>

Sincerely yours,

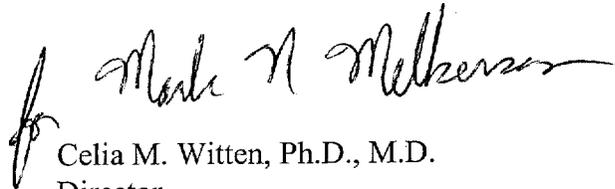

Celia M. Witten, Ph.D., M.D.  
Director  
Division of General, Restorative and  
Neurological Devices  
Office of Device Evaluation  
Center for Devices and  
Radiological Health

Enclosure

510(k) Number (if known): K021359

Device Name: Digi-Pro TENS / Model: WL-2203, WL-2204, WL-2205

**Indications For Use (Available for WL-2203 & 'TENS function' of WL-2205):**

This device is a prescription device and only for symptomatic relief of chronic intractable pain.

**Indications For Use (Available for WL-2204 & 'EMS function' of WL-2205):**

- Relaxation of muscle spasms.
- Prevention or retardation of disuse atrophy.
- Increasing local blood circulation.
- Muscle re-education.
- Immediate post-surgical stimulation of calf muscles to prevent venous thrombosis.
- Maintaining or increasing range of motion.

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE IF NEEDED)

---

Concurrence of CDRH, Office of Device Evaluation (ODE)

*for Mark N. Melburn* (Optional Format 3-10-98)  
(Division Sign-Off)

Division of General, Restorative  
and Neurological Devices

510(k) Number K021359