

DEC - I 2006

K063220

7

Section II

510(k) SUMMARY

This summary of 510(k) safety and effectiveness information is submitted in accordance with the requirements of SMDA 1990 and 21 CFR 807.92.

510(k) Number:

Date	19 October 2006
Submitter	Intuitive Surgical, Inc. 950 Kifer Road Sunnyvale, CA 94086
ER Number	2955842
Contact	Jerry Tsutsumi Sr. Regulatory Engineer Telephone: (408) 523 - 2415 Fax: (408) 523 - 1390 e-mail: jerry.tsutsumi@intusurg.com
Subject Device	<u>Name:</u> <i>Intuitive Surgical® da Vinci® S™</i> Surgical System (Model IS2000, V1.1) and <i>EndoWrist®</i> Endoscopic Instruments. <u>Classification Name:</u> System, Surgical, Computer Controlled Instrument (21 CFR 876.1500) <u>Common Name:</u> Endoscopic Instrument Control System, Endoscopic Instruments, and accessories
Predicate Devices	<i>Intuitive Surgical da Vinci S</i> Surgical System (Model IS2000) and <i>EndoWrist</i> Endoscopic Instruments (legally marketed under K050369, K021036, K050404 and K050802).
Device Description	The <i>da Vinci S</i> Surgical System, Model IS2000 V1.1, consists of three integrated sub-systems as follows: <u>Intuitive Surgical Endoscopic Instrument Control System:</u> The Endoscopic Instrument Control System is comprised of two sub-systems - the Surgeon Console, Model SS2000, and Patient Side Cart, Model PS2000. While seated at the Surgeon Console, the surgeon controls critical aspects of the procedure, including movement of the endoscopic instruments and endoscope, within the operative field. Endoscopic instrument and camera movements are controlled by the surgeon through use of the Master Tool Manipulators (MTM), two hand operated mechanisms residing within the Surgeon Console.

**Device
Description
(continued)**

The endoscopic instruments are held in a fixed position (with respect to the patient) by either two (or optionally three) unique manipulators known as Patient Side Manipulators (PSM), which are located on the Patient Side Cart (PSC, Model PS2000). The endoscope is also held in a fixed position (with respect to the patient) by another manipulator, similar to the PSM, known as the Endoscope Camera Manipulator (ECM) and also located on the PSC. The PSM and ECM are attached to surgical arms on the PSC known as Set-up Joint (SUJ) arms. Commands from the Surgeon Console are relayed to the PSC, which is located immediately adjacent to the patient, via a cable. Instrument and endoscope changes are performed by another provider positioned adjacent to the PSC.

Intuitive Surgical Stereo View Endoscopic System: The endoscopic vision system used with the da Vinci Surgical System, also known as Intuitive Surgical *Insite*[®] Vision System, Model VS2000, consists of a stereo endoscope, endoscopic camera, and various accessories, including a light source and light guides. The *Insite* Vision System provides two independent images that are relayed to the viewer located in the Surgeon Console, where they are fused to form a 3-D (or alternatively a 2-D image) image of the surgical field.

Intended Use

The Intuitive Surgical Endoscopic Instrument Control System is intended to assist in the accurate control of Intuitive Surgical Endoscopic Instruments including rigid endoscopes, blunt and sharp endoscopic dissectors, scissors, scalpels, ultrasonic shears, forceps/pick-ups, needle holders, endoscopic retractors, stabilizers, electrocautery and accessories for endoscopic manipulation of tissue, including grasping, cutting, blunt and sharp dissection, approximation, ligation, electrocautery, suturing and delivery and placement of microwave ablation probes and accessories during urologic surgical procedures, general laparoscopic surgical procedures, gynecological laparoscopic surgical procedures, general non-cardiovascular thoracoscopic surgical procedures, and thoracoscopically assisted cardiomy procedures. The system can also be employed, with adjunctive mediastinotomy to perform coronary anastomosis during cardiac revascularization. The system is indicated for adult and pediatric use. It is intended for use by trained physicians in an operating room environment in accordance with the representative specific procedures set forth in the Professional Instructions for Use.

**Comparison to
Predicate
Device**

This 510(k) notification is submitted for design modifications to the Endoscopic Instrument Control System, and Vision System.

The modifications to the Vision System Cart (Model VS2000) consist of an optional, enhanced endoscopic camera and Camera Control Units (CCU), and an optional, touch screen display. The touch screen display on the Vision System Cart provides redundant video capabilities as the touch screen display that is currently on the Patient Side Cart (Model PS2000), and the updated endoscopic camera and Camera Control Units provide enhanced vision system performance. An optional still/video capture device (DVD Recorder) will be available and auxiliary control will be provided with the touch screens.

The modifications to the Endoscopic Instrument Control System consist of primarily software modifications to support new features as follows:

Instructional Telestration capabilities: instructional controls and additional controls duplicating some of the Surgeon's Console Left-Side Pod controls (camera calibration and camera set-up functions).

The addition of ECM LED's (Light Emitting Diode's) as fault indicators for User Interface improvements, identical to current PSM LED's functionality. An improved ECM "under-drape Cannula Mount", with a new ECM drape configuration, and ECM cannula sensing for User Interface improvements.

The Surgeon Console is updated with activation of a foot pedal for energy activation of a bipolar and/or a monopolar instrument, with separate bipolar/monopolar connections integrated into the rear IO panel of the Surgeon Console

The user interface design is essentially identical to the predicate device except for minor modifications to accommodate the aforementioned changes.

Device operation, functionality, and methods of use for the subject device are identical to the predicate device. The technology, materials, manufacturing methods, and performance are essentially the same for the predicate device as the subject device.

**Technological
Characteristics**

The technological characteristics of the subject devices are essentially the same as for the predicate devices.

**Performance
Data**

Design analysis and comparison, as well as bench testing and risk analysis activities, have been conducted to confirm that the characteristics of the modified device are substantially equivalent to the predicate devices cited.

Conclusion

Based upon the device's general specifications, intended use, and results of risk analysis and performance testing provided in this pre-market notification, the *da Vinci S* Surgical System described herein has been shown to be substantially equivalent to current legally marketed predicate device.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

Intuitive Surgical, Inc.
% Mr. Michael H. Yramategui
Senior Director, Regulatory Affairs
and Quality Assurance
950 Kifer Road
Sunnyvale, California 94086

DEC - 1 2006

Re: K063220

Trade/Device Name: *Intuitive Surgical*[®] Endoscopic Instrument Control System
Regulation Number: 21 CFR 876.1500
Regulation Name: Endoscope and accessories
Regulatory Class: II
Product Code: NAY
Dated: October 20, 2006
Received: October 24, 2006

Dear Mr. Yramategui:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); good manufacturing practice requirements as set


Page 2 – Mr. Michael H. Yramategui

forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

This letter will allow you to begin marketing your device as described in your Section 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please contact the Office of Compliance at (240) 276-0115. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). You may obtain other general information on your responsibilities under the Act from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (240) 276-3150 or at its Internet address <http://www.fda.gov/cdrh/industry/support/index.html>.

Sincerely yours,



Mark N. Melkerson
Director
Division of General, Restorative
and Neurological Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

Indications for Use

510(k) Number (if known):

Device Name: *Intuitive Surgical*[®] Endoscopic Instrument Control System

Indications For Use:

The *Intuitive Surgical* Endoscopic Instrument Control System is intended to assist in the accurate control of *Intuitive Surgical* Endoscopic Instruments including rigid endoscopes, blunt and sharp endoscopic dissectors, scissors, scalpels, ultrasonic shears, forceps/pick-ups, needle holders, endoscopic retractors, stabilizers, electrocautery and accessories for endoscopic manipulation of tissue, including grasping, cutting, blunt and sharp dissection, approximation, ligation, electrocautery, suturing, and delivery and placement of microwave ablation probes and accessories during urologic surgical procedures, general laparoscopic surgical procedures, gynecological laparoscopic surgical procedures, general non-cardiovascular thoracoscopic surgical procedures, and thoracoscopically assisted cardiomy procedures. The system is indicated for adult and pediatric use. The system can also be employed, with adjunctive mediastinotomy to perform coronary anastomosis during cardiac revascularization. It is intended for use by trained physicians in an operating room environment in accordance with the representative specific procedures set forth in the Professional Instructions for Use.


Prescription Use X
(Part 21 CFR 801 Subpart D)

AND/OR

Over-The-Counter Use _____
(21 CFR 807 Subpart C)

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDRH, Office of Device Evaluation (ODE)

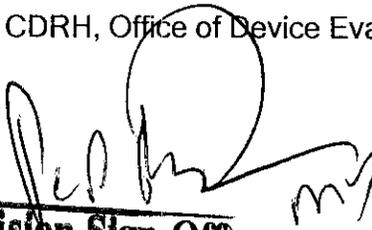
(Division Sign-Off)
**Division of General, Reconstructive
and Neurological Devices**

510(k) Number 1Ld3220

Page 1 of 1