



K081079

MAY - 2 2008

5. 510(K) SUMMARY

Date prepared	April 2, 2008
Name	SenoRx, Inc. 11 Columbia Aliso Viejo, CA 92656 T. 949.362.4800; F. 949.362.0300
Contact person	Eben Gordon Vice President, RA/QA SenoRx, Inc. T. 949.362.4800; F. 949.362.0300
Device name	Contura MLB Source Applicator for Brachytherapy
Common name	Multi-Lumen balloon source applicator
Classification name	Remote controlled radionuclide source applicator
Classification regulation	21 CFR 892.5700; 90 JAQ
Predicate devices	SenoRad Multi-Lumen Balloon Source Applicator for Brachytherapy (K071229) MammoSite Radiation Therapy System (K030558)
Description	The Contura MLB Applicator consists of a multi-lumen catheter connected to an inflatable spherical balloon that can be attached to commercially available High Dose Rate remote afterloader equipment for passage of the radiation source delivery wire. Five radiation source wire lumens are provided; one central lumen located along the long axis of the applicator and four lumens symmetrically offset from the central lumen. The balloon is inflated to a 4.5 - 6 cm spherical shape by a controlled volume injection of a saline/contrast solution.
Indications for use	The Contura Multi-Lumen Balloon Source Applicator for Brachytherapy is intended to provide brachytherapy when the physician chooses to deliver intracavitary radiation to the surgical margins following lumpectomy for breast cancer.
Summary of substantial equivalence	Preclinical studies demonstrated that the Contura MLB Applicator performed as intended under simulated use conditions. The dosimetry of the Contura MLB Applicator and the predicate devices demonstrated that the Contura MLB Applicator could deliver an equivalent radiation dose. In summary, the Contura MLB Applicator as described in this submission is substantially equivalent to the predicate devices.



Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

MAY - 2 2008

SenoRx, Inc.
% Mr. Mark Job
Responsible Third Party Official
Regulatory Technology Services, LLC
1393 25th Street NW
BUFFALO MN 55313

Re: K081079

Trade/Device Name: Contura Multi-Lumen Balloon Source Applicator for Brachytherapy
Regulation Number: 21 CFR 892.5700
Regulation Name: Remote controlled radionuclide applicator system
Regulatory Class: II
Product Code: JAQ
Dated: April 15, 2008
Received: April 16, 2008

Dear Mr. Job:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act and the limitations described below. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

The Office of Device Evaluation has determined that there is a reasonable likelihood that this device will be used for an intended use not identified in the proposed labeling and that such use could cause harm. Therefore, in accordance with Section 513(i)(1)(E) of the Act, the following limitation must appear in the Warnings section of the device's labeling:

The safety and effectiveness of the Contura Multi-Lumen Balloon Source Applicator for Brachytherapy as a replacement for whole breast irradiation in the treatment of breast cancer has not been established.

The Warning must be presented within a black box, and the font should be bold and the same size as any surrounding text. The Warning should be the first item in your list of warnings.

Please note that the above labeling limitations are required by Section 513(i)(1)(E) of the Act. Therefore, a new 510(k) is required before these limitations are modified in any way or removed from the device's labeling.

The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and permits your device to proceed to the market. This letter will allow you to begin marketing your device as described in your Section 510(k) premarket notification if the limitation statement described above is added to your labeling.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

If you desire specific information about the application of other labeling requirements to your device (21 CFR Part 801), please contact the Office of Compliance at (240) 276-0100. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR Part 807.97). You may obtain other general information on your responsibilities under the Act from the Division of Small Manufacturers, International, and Consumer Assistance at its toll-free number (800) 638-2041 or (240) 276-3150 or at its Internet address <http://www.fda.gov/cdrh/industry/support/index.html>.

Sincerely yours,



Donna-Bea Tillman, Ph.D., M.P.A.

Director

Office of Device Evaluation

Center for Devices and Radiological Health

Enclosure

4. INDICATIONS FOR USE

510(k) Number (if known): K081079

Device Name: _____ Contura Multi-Lumen Balloon Source Applicator for Brachytherapy _____

Indications for Use:

The Contura Multi-Lumen Balloon Source Applicator for Brachytherapy is intended to provide brachytherapy when the physician chooses to deliver intracavitary radiation to the surgical margins following lumpectomy for breast cancer.


Prescription Use X
(Part 21 CFR 801 Subpart D)

AND/OR

Over the Counter Use _____
(21 CFR 801 Subpart C)

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE OF NEEDED)

Concurrence of CDRH, Office of Device Evaluation (ODE)

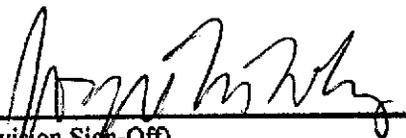

(Division Sign-Off)
Division of Reproductive, Abdominal,
and Radiological Devices

510(k) Number K081079

Page __ of __