



DEC 19 2008

The Binding Site Ltd.
c/o Mr. Jay H. Geller
West Tower, Suite 4000
2425 West Olympic Boulevard
Santa Monica, California 90404

Re: k081827

Trade/Device Name: Human IgA Liquid Reagent Kit for use on SPA_{PLUS}TM
Regulation Number: 21 CFR 866.5510
Regulation Name: Immunoglobulins A, G, M, D, E Immunological Test System
Regulatory Class: Class II
Product Code: CFN
Dated: June 23, 2008
Received: August 27, 2008

Dear Mr. Geller:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to such additional controls. Existing major regulations affecting your device can be found in Title 21, Code of Federal Regulations (CFR), Parts 800 to 895. In addition, FDA may publish further announcements concerning your device in the Federal Register.


Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Parts 801 and 809); and good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820). This letter

Page 2 – The Binding Site, Ltd.

notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please contact the Office of In Vitro Diagnostic Device Evaluation and Safety at (240) 276-0450. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). For questions regarding postmarket surveillance, please contact CDRH's Office of Surveillance and Biometric's (OSB's) Division of Postmarket Surveillance at (240) 276-3474. For questions regarding the reporting of device adverse events (Medical Device Reporting (MDR)), please contact the Division of Surveillance Systems at (240) 276-3464. You may obtain other general information on your responsibilities under the Act from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (240) 276-3150 or at its Internet address <http://www.fda.gov/cdrh/industry/support/index.html>.

Sincerely yours,

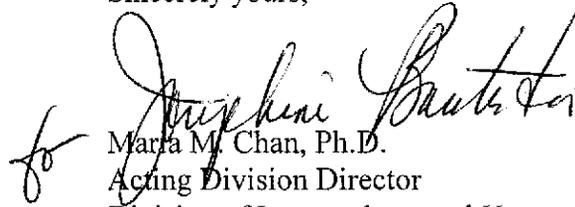

Marla M. Chan, Ph.D.

Acting Division Director

Division of Immunology and Hematology Devices

Office of In Vitro Diagnostic Device Evaluation
and Safety

Center for Devices and Radiological Health

Enclosure

Indications for Use

510(k) Number (if known): K081827

Device Name: Human IgA liquid reagent kit for use on SPA_{PLUS}TM

Indications for Use: This kit is intended for the quantitative *in vitro* determination of human IgA in serum, lithium heparin or EDTA plasma, using the Binding Site SPA_{PLUS}TM turbidimetric analyser. Measurement of IgA aids in the diagnosis of abnormal protein metabolism and the body's lack of ability to resist infectious agents. The test results are to be used in conjunction with other clinical and laboratory findings.


Prescription Use
 (Part 21 CFR 801 Subpart D)

AND/OR

Over-The-Counter Use
 (21 CFR 801 Subpart C)

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE
OF NEEDED)

Concurrence of CDRH, Office of Device Evaluation (ODE)

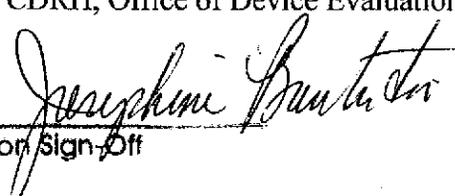
Division Sign-Off

Page 1 of 1

Office of In Vitro Diagnostic
Device Evaluation and Safety

510(k) 081827

0 14