

# NovoPen® 3 Demi

Dial-A-Dose  
Insulin Delivery System  
Instructions For Use



Notex - Tryk & Design as

Order no. 128826

NovoPen 3 Demi, USA


3. proof 00-10-26.

**Novo Nordisk**




Corrections on this page = ◆◆◆


### NovoPen® 3 Demi Insulin Delivery Device

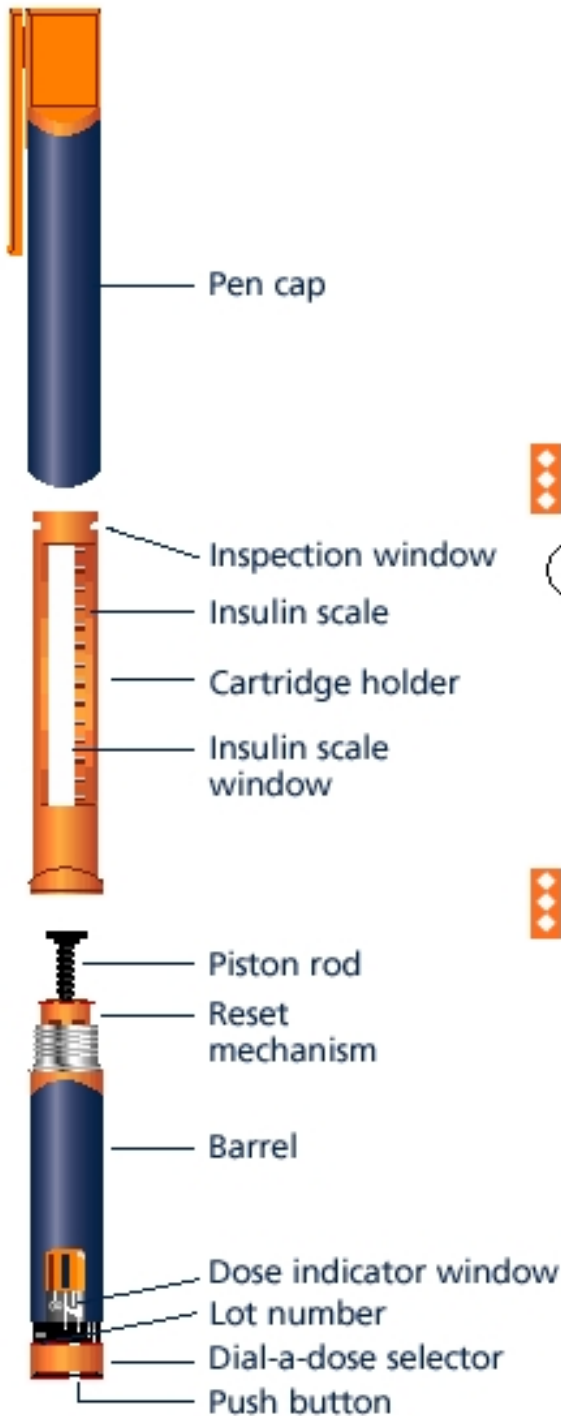

### NovoFine® Disposable Needle

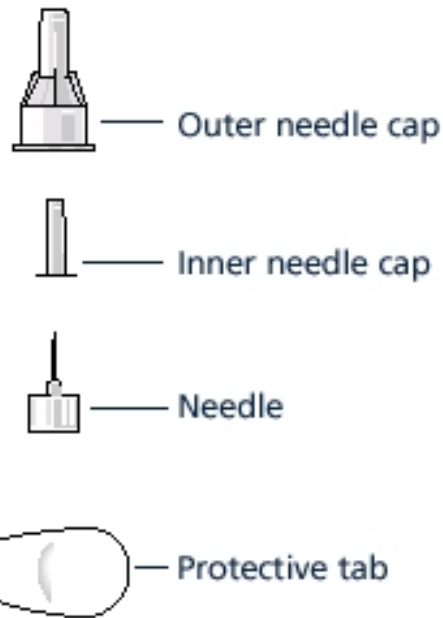

### PenFill® Cartridge (3 mL)

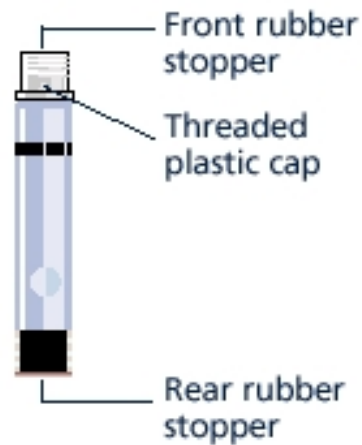

Need Help?  
Call 1-800-727-6500

# 4 **NovoPen<sup>®</sup> 3 Demi Instruction Manual**

## 5 6 **Dial-A-Dose Insulin Delivery System**

### 7 8 **INTRODUCTION**

9  
10  
11  
12  
13 NovoPen<sup>®</sup>3 Demi delivers a minimum dose of 1 unit to a maximum dose of 35  
14 units of insulin in half unit steps. A raised circle on the push button makes it easy  
15 for you to know your NovoPen 3 Demi from the ordinary NovoPen 3. This booklet  
16 includes everything you need to know about using the NovoPen 3 Demi. Please  
17 read it carefully before using your NovoPen 3 Demi for the first time.

18  
19 The NovoPen 3 Demi is designed for use with:

- 20 ■ PenFill<sup>®</sup> 3 mL cartridges.
- 21 ■ NovoFine<sup>®</sup> disposable needles.

22 **NovoFine disposable needles are for single-use only.**

23 You will also need alcohol swabs.

24  
25 If you have any questions about your NovoPen 3 Demi insulin delivery system,  
26 please call Novo Nordisk Pharmaceuticals, Inc. at 1-800-727-6500.

27  
28 **Please complete and return the NovoPen 3 Demi warranty card.**

29  
30  
31  
32 See **Important Things to Know** and **Important Notes** on pages 33-35.

33  
34

35 **HOW TO USE THIS BOOKLET**

36

37 **This booklet gives you step-by-step instructions for using the NovoPen 3**  
38 **Demi.**

39

40 Begin by reviewing the drawing layout of the parts of the NovoPen 3 Demi,  
41 PenFill 3 mL cartridge, and NovoFine disposable needle. The inside front cover  
42 opens out so you have a handy reference while you read the rest of the booklet.

43

44 Most pages contain a drawing on the right with numbered instructions to the left  
45 of the drawing.

46 **Important additional information is given below the drawing.**

47

48 We suggest that you **read the text and look at the drawing** to make sure that  
49 you understand each step thoroughly.

50

51

52

53

54

55

56

57

58

59

60

61

62

63

64

65

66

67

68

69

70

71

72

73

74

75

76

77


78

79	<b>TABLE OF CONTENTS</b>	
80		
81	SECTION 1:	
82	Preparing the NovoPen 3 Demi.....	5
83		
84	SECTION 2:	
85	Inserting the PenFill 3 mL Cartridge.....	8
86		
87	SECTION 3:	
88	Attaching the NovoFine Disposable Needle.....	12
89		
90	SECTION 4:	
91	Doing an Air Shot .....	16
92		
93	SECTION 5:	
94	Giving the Injection .....	20
95		
96	SECTION 6:	
97	Removing the NovoFine Disposable Needle.....	24
98		
99	SECTION 7:	
100	Removing the PenFill 3 mL Cartridge.....	26
101		
102	FUNCTION CHECK .....	28
103		
104	STORAGE.....	31
105		
106	MAINTENANCE.....	32
107		
108	IMPORTANT THINGS TO KNOW.....	33
109		
110	IMPORTANT NOTES.....	34
111		
112	WHAT TO DO IF.....	36
113		
114	WARRANTY .....	37
115		

116 **SECTION 1**            **Preparing the NovoPen 3 Demi**  
117

118 **Remove the device cap:**

- 119     1. Remove the NovoPen 3 Demi from the case.  
120     2. Gently twist the pen cap until the cap separates from the barrel.  
121     3. Pull the pen cap straight up to remove it.  
122

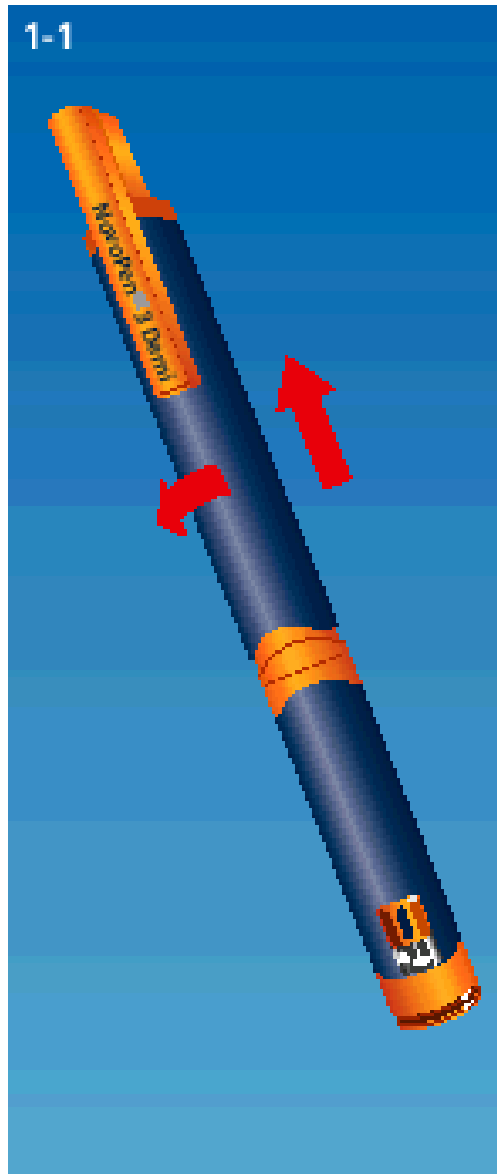

Need Help?  
Call 1-800-727-6500

123  
124  
125 **If you use more than one insulin product (such as Novolin® R, Novolin® N,**  
126 **Novolin® 70/30, or NovoLog®), use a separate insulin delivery device for each**  
127 **product.**

128

129 **SECTION 1 (cont.)**

130

131 **Separate the cartridge holder from the barrel:**

132

- 133 4. Unscrew and remove the cartridge holder from the barrel.

134



135


136

137 **Make sure the dose indicator window shows zero:**

138

- 139 5. Press the push button all the way in until zero (0) appears in the window.  
140 The zero should be lined up with the stripe below the dose indicator  
141 window.

142

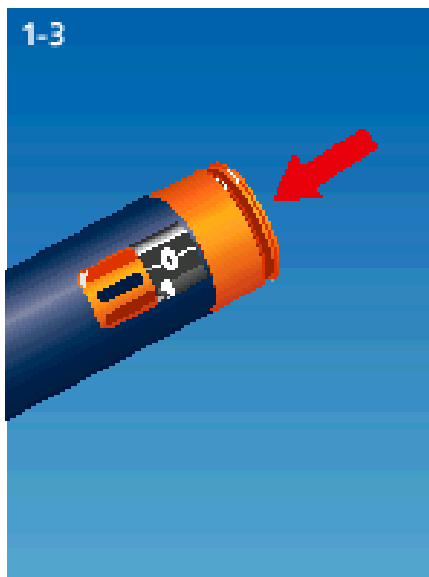

143






145  
146  
147  
148  
149  
150  
151  
152  
153  
154  
155

**SECTION 1 (cont.)**

The end of the piston rod should be flat against the end of the reset mechanism prior to inserting each new PenFill 3 mL cartridge. It should not be sticking out.

**If the piston rod is sticking out:**

Turn the end of the reset mechanism in a clockwise direction until it is no longer sticking out. Never push the piston rod back in.

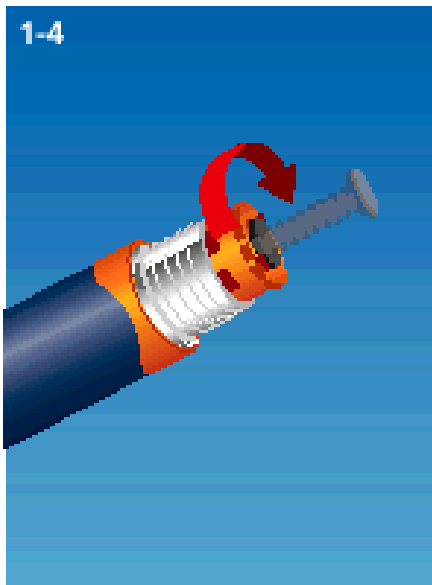

156




157  
158  
159  
160  
161  
162  
163  
164  
165  
166

You should never reset the piston rod until it is time to remove the used PenFill 3 mL cartridge and insert a new one.

If the reset mechanism locks, it is usually due to improper technique. Gently turn the mechanism side to side until it unlocks. Then call our toll free number (1-800-727-6500) so that we may go over your technique with you.

167 **SECTION 2                    Inserting the PenFill 3 mL Cartridge**  
168

- 169 1. To remove the PenFill cartridge from its wrapper, push the cartridge  
170 through the foil side of the packaging. Always make sure that the PenFill  
171 cartridge you use contains the correct type of insulin (such as Novolin R,  
172 Novolin N, Novolin 70/30, or NovoLog). If you are treated with more than  
173 one type of insulin in PenFill cartridges, you should use a separate insulin  
174 delivery device for each type of insulin. Before use, check that the PenFill  
175 cartridge is full and intact. If not, do not use it.  
176

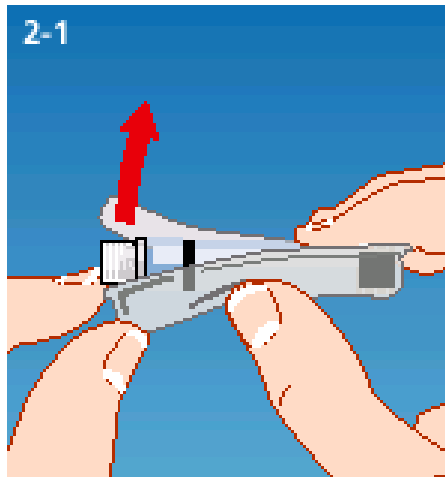

- 177  
178  
179 2. In the PenFill Information For The Patient leaflet, you will find instructions  
180 on how to prepare the insulin if the PenFill contains a suspension insulin  
181 (white and cloudy) such as Novolin N or Novolin 70/30.  
182  
183

184 Each PenFill 3 mL cartridge contains a total of 300 units of insulin. Make sure  
185 you are using the correct type of insulin. On the glass part of the cartridge is the  
186 name of the insulin.

187  
188 Each PenFill cartridge is for single-person use only. DO NOT share the same  
189 cartridge with anyone even if you attach a new disposable needle for each  
190 injection. Sharing the cartridge can spread disease.

191 **Use only a new PenFill 3 mL cartridge when loading the NovoPen 3 Demi.**

192 **Never load a partially filled cartridge.**


193 **Never try to refill a used PenFill 3 mL cartridge.**  
194  
195

196  
197  
198  
199  
200  
201  
202  
203  
204

**SECTION 2 (cont.)**

**Insert the PenFill cartridge:**

2. Hold the cartridge holder so the wider opening is up.
3. Drop the PenFill cartridge into the cartridge holder, plastic cap first.

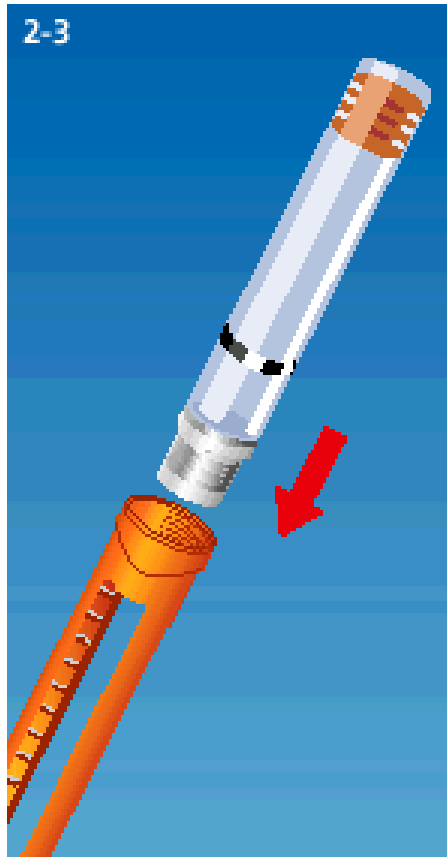

205  
206  
207  
208  
209  
210  
211

A threaded plastic cap surrounds the end of the PenFill® cartridge, like the cap on a bottle. In the center is the front rubber stopper.

The rear rubber stopper is at the other end of the PenFill cartridge.

212 **SECTION 2 (cont.)**


213

214 **Re-attach the cartridge holder:**

215

216 4. Screw the barrel into the cartridge holder completely until it is tight.

217

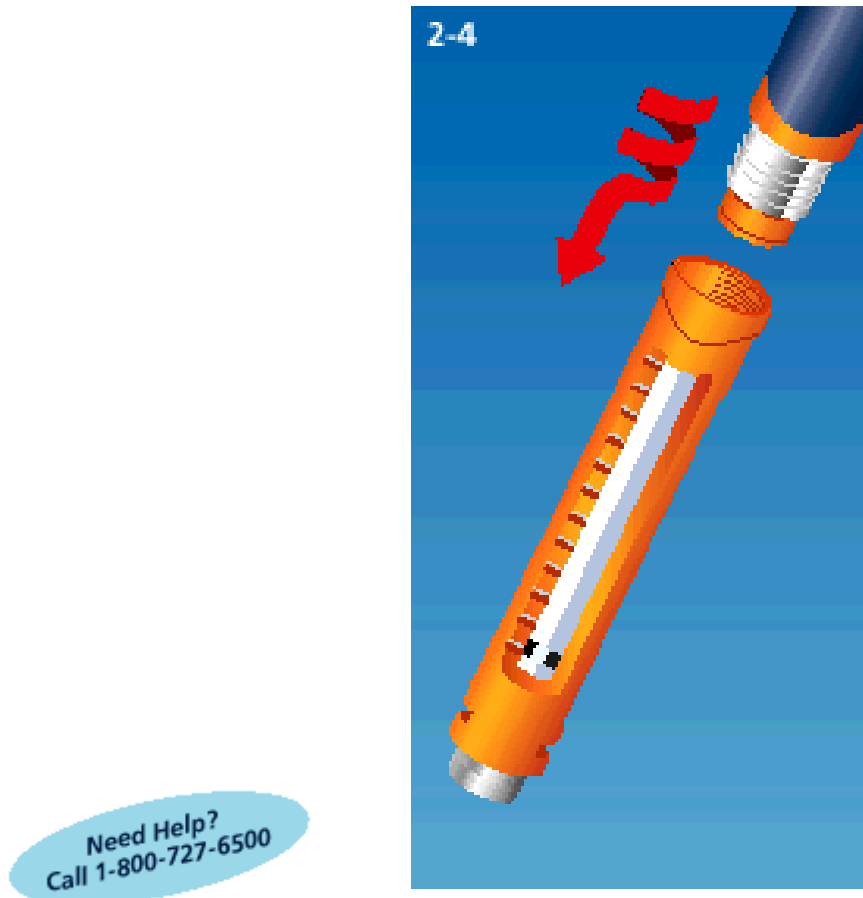

218

219

220

221

222 You can see the cartridge in the insulin scale window. The cartridge holder has a  
223 scale with marks showing about how much insulin is left in the PenFill cartridge.

224

225

226

227 **SECTION 3 Attaching the NovoFine® Disposable Needle**  
228


229 At the end of the cartridge holder are two inspection windows. You can see the  
230 cartridge through these windows.  
231

232 **If you use a suspension insulin (white and cloudy) such as Novolin® N or**  
233 **Novolin® 70/30, use the windows to check if there is enough insulin left for**  
234 **proper mixing.** (see below)  
235

236 **Check the amount of insulin remaining:**

- 237 ■ If the rear rubber stopper cannot be seen in the inspection window, you have  
238 enough insulin for mixing left in the cartridge.
- 239 ■ If the rear rubber stopper can be seen in the inspection window, you do not  
240 have enough insulin left in the cartridge and must insert a new PenFill 3 mL  
241 cartridge.  
242

243 See Section 7 for instructions on removing a PenFill cartridge and Section 2 for  
244 inserting a new one.  
245

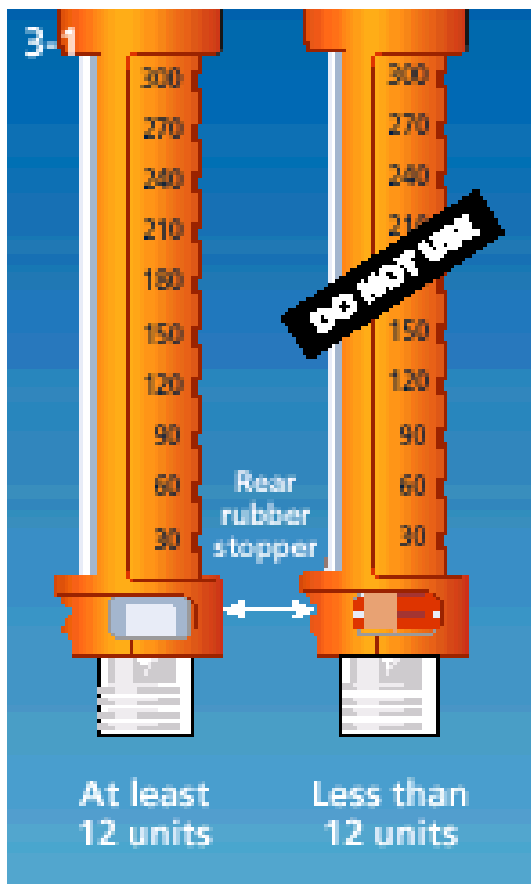



249 **SECTION 3 (cont.)**


250

251 **For users of suspension insulin (white and cloudy) such as Novolin N or**  
252 **Novolin 70/30:**

253

254 **Always remix the insulin before each injection.**

255 To remix the insulin, turn the NovoPen 3 Demi up and down between positions **A**  
256 and **B** 10 times or until the insulin looks uniformly white and cloud  
257

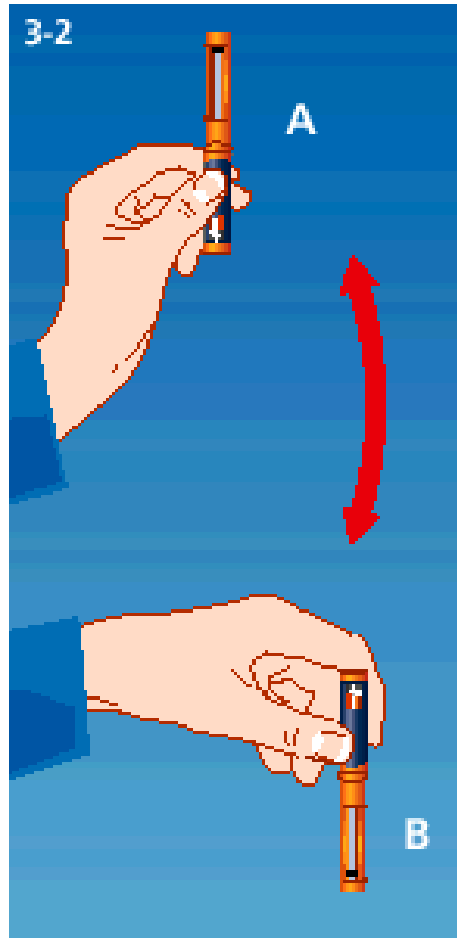

Need Help?  
Call 1-800-727-6500

258

259

260


261



262  
263  
264  
265

**SECTION 3 (cont.)**

1. Wipe the front rubber stopper with an alcohol swab.

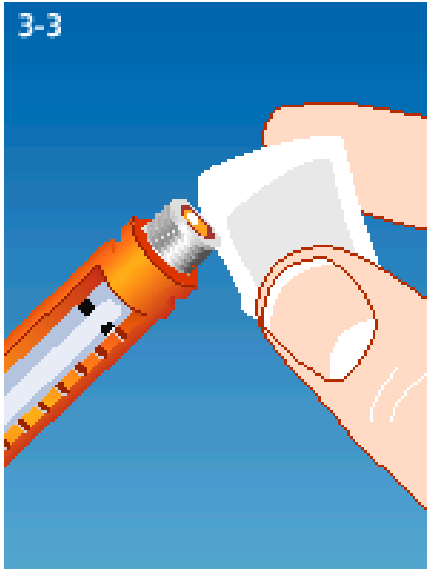


266  
267  
268  
269  
270  
271

You must wipe the front rubber stopper with an alcohol swab before each injection, even if you are using the same PenFill cartridge.

272 **SECTION 3 (cont.)**

273  
274  
275  
276  
277

2. Remove the protective tab from the NovoFine disposable needle.
3. Screw the NovoFine disposable needle firmly onto the PenFill 3 mL cartridge until it is tight.

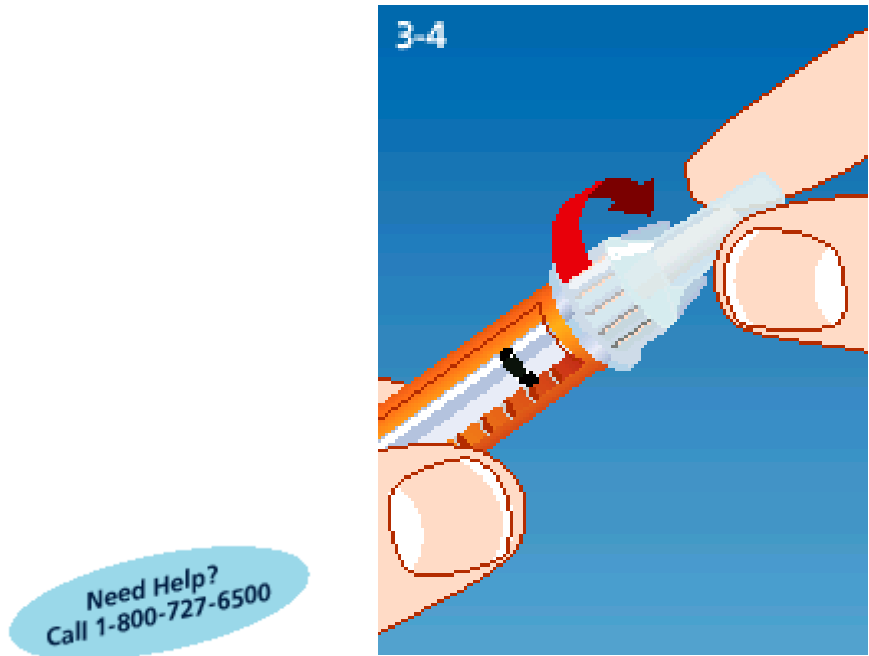

278  
279  
280  
281  
282  
283  
284  
285

Never place a NovoFine disposable needle on your NovoPen 3 Demi until you are ready to do an air shot and give an injection. If the NovoFine needle is left on, some liquid may leak out of the PenFill cartridge. This may cause a change in the strength of the suspension insulin such as Novolin N or Novolin 70/30.

286

287 **SECTION 4                    Doing an Air Shot**

288

289 The PenFill cartridge may contain an air bubble, and small amounts of air may  
290 collect in the needle and PenFill cartridge when you use them. To avoid injecting  
291 air and to ensure proper dosing, you must perform an air shot before each  
292 injection.

293

294 **Before doing the air shot, the dose indicator window must show zero (0).**

295

296 If you use a suspension insulin, such as Novolin N or Novolin 70/30 and have  
297 used the PenFill cartridge for previous injections, make sure there is enough  
298 insulin left in the PenFill cartridge to properly mix the insulin (see page 12). If  
299 there is enough insulin left in the PenFill cartridge, see the next page for  
300 instructions.

301

302 16

303 **SECTION 4 (cont.)**

304

305 **Set the NovoPen 3 Demi for the air shot:**

306

- 307 1. Turn the dial-a-dose selector to 2 units. Full units are shown as numbers.  
308 Half units are shown as long lines between the numbers.  
309



Need Help?  
Call 1-800-727-6500

310

311

312 **If you dial more than 2 units, DO NOT turn the dial back to zero (0).** If you  
313 do, the extra insulin will squirt out of the needle. You may complete the air shot  
314 with the number of units you have dialed or refer to Section 5 on page 21 for  
315 instructions on how to reset the dose to zero.

316

317 **SECTION 4 (cont.)**

318

319 **Uncap the NovoFine needle:**

320

321 2. Pull off the outer needle cap and set aside.

322 3. Pull off the inner needle cap and discard.

323

324 Do not use the needle if it is bent or damaged.

325



326

327

328 4. Hold the NovoPen 3 Demi with the NovoFine needle pointing up.

329 5. Tap the cartridge holder with your finger a few times to raise any air  
330 bubbles that may be present to the top of the cartridge.

331



332

333

334 **SECTION 4 (cont.)**

335

336 **Do the air shot:**

337

338 6. Press the push button all the way in. A drop of insulin should appear at the  
339 needle tip.

340

341 **If no insulin appears, repeat the following steps, until a drop of insulin**  
342 **appears:**

343

344 a. Make sure the NovoFine needle is securely attached.

345 b. Dial 2 units.


346 c. Tap the cartridge holder with your finger.

347 d. Press the push button all the way in.

348

349 There may still be some small air bubble(s) in the PenFill cartridge after this, but  
350 they will not affect your dose and they will not be injected.

351

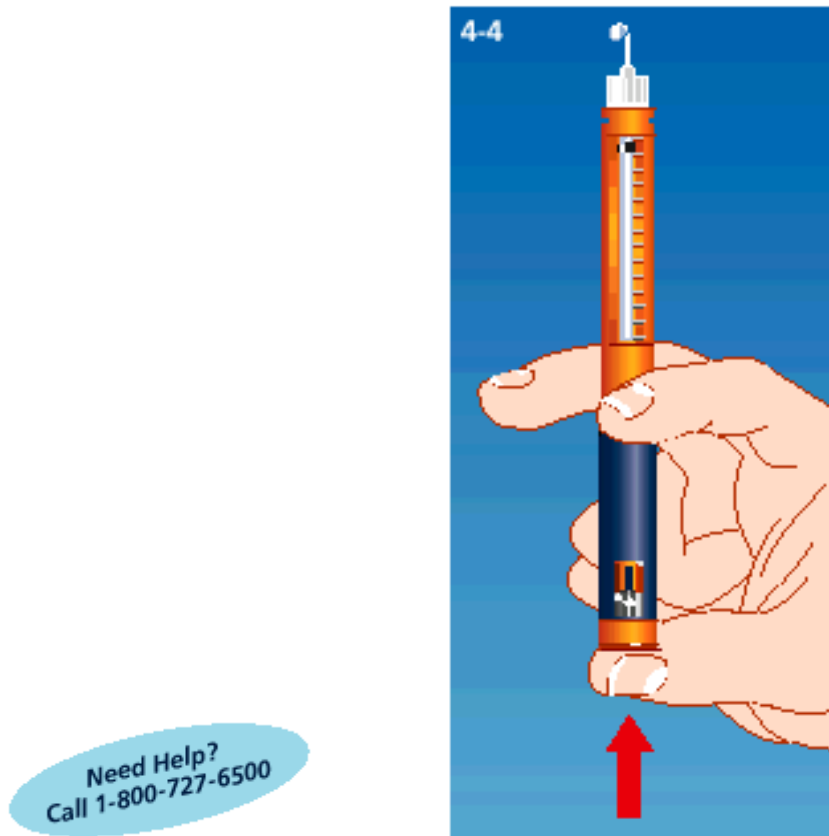

352

353

354 When you press the push button, the piston rod presses against the rear rubber  
355 stopper. This moves the rear rubber stopper and pushes the correct amount of  
356 insulin up through the needle.



358 **SECTION 5 Giving the Injection**

359

360 **Be sure to do an air shot before giving each injection (see pages 16-19).**

361

**Select the dose:**

362

363

1. Check that the dial-a-dose selector is set to zero. If not, follow the instructions on the next page. Turn the dial-a-dose selector until you see the correct number of units in the dose indicator window. Full units are shown as numbers. Half units are shown as long lines between the numbers.

364

365

366

367

368

369

**DO NOT use the clicking sound as a guide for selecting your dose.**

370



371

372

373

The NovoPen 3 Demi can deliver insulin in half unit steps from a minimum dose of 1 unit to a maximum dose of 35 units.

374

375

376

**If you dial more than your dose, DO NOT turn the dial back to zero (0).** If you do, the extra insulin will squirt out of the needle. For instructions on how to reset the dose to zero (0) so you can start again, see the next page.

377

378

379

380

381



382 **SECTION 5 (cont.)**


383

384 If you dial a larger dose than you need, pull the barrel and the cartridge holder  
385 apart, as shown in the drawing **A**. While holding them apart, gently press the  
386 push button against a hard surface and release your grip **B**. Your dose indicator  
387 window should be back to zero (0).

388

389 You can now dial the correct number of units.

390

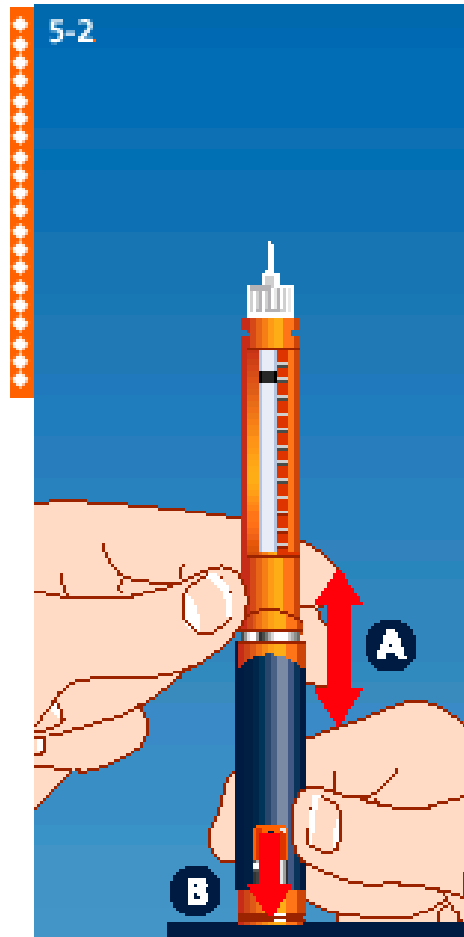

391

392

393

394 **SECTION 5 (cont.)**

395

396 **Giving the injection:**

397

398

399

400

401

402

403

404

405

406

407

408

409

410

411

412

413

2. After the air shot is done and you have chosen the correct number of units, insert the NovoFine needle in the correct injection site on your body. (Use the injection technique recommended by your health care professional). If you use a suspension insulin such as Novolin N or Novolin 70/30, mix the insulin (see page 13, Section 3) and make sure the insulin looks uniformly white and cloudy before you inject.

3. Press the push button **as far as it will go** to deliver the insulin. Do not force it.

To ensure that all the insulin is injected, keep the NovoFine needle in the skin for several seconds after the injection with your thumb on the push button. Keep the push button fully depressed until after the NovoFine needle has been withdrawn.

**Important: Never turn the dial-a-dose selector to inject the insulin.**



414

415

416

417

When you get near the end of a PenFill cartridge, you may need to give yourself two injections to receive your full dose. Check the dose indicator window after

418 giving an injection. If zero does not appear in the dose indicator window, you did  
419 not receive your full dose. See the next page for instructions on how to get the  
420 remaining part of your dose.  
421 22

422  
423  
424  
425  
426  
427  
428  
429  
430  
431  
432  
433  
434  
435  
436  
437  
438  
439  
440  
441  
442  
443  
444  
445  
446  
447

**SECTION 5 (cont.)**

**4. Check the dose indicator window to make sure it shows zero (0). If zero does not appear, you did not receive the full dose.**

If the dose indicator window does not show zero, there were not enough units of insulin in the PenFill cartridge for you to receive the full dose. The dose indicator window shows the number of units that you did not receive.

For example, if you dial **25** units and there are only **20** units left in the PenFill cartridge, after the injection the number in the dose indicator window will be **5** ( $25-20 = 5$ ). If this happens, proceed with the following steps to get the remaining part of your dose:

- a. Note the number of units in the dose indicator window.
- b. Remove the NovoFine needle (see Section 6).
- c. Remove the empty PenFill 3 mL cartridge (see Section 7).
- d. Insert a new PenFill 3 mL cartridge (see Section 2).
- e. Attach a NovoFine needle (see Section 3).
- f. Do an air shot (see Section 4).
- g. Dial the number of units noted in step a.
- h. Give the injection.



448  
449  
450

451 **SECTION 6 Removing the NovoFine Disposable Needle**

452

453 **Remove the NovoFine disposable needle:**

454

455 1. After the injection, remove the needle without replacing the cap.

456

457 2. Hold the cartridge holder firmly while you unscrew the NovoFine  
458 disposable needle.

459

460 3. Place the NovoFine disposable needle in a puncture-resistant disposable  
461 container.

462

463 Health care professionals, relatives, and other caregivers should also follow the  
464 above instructions to eliminate the risk of unintended needle penetration.

465

466

467

468 **The NovoFine disposable needle must be removed immediately after each**  
469 **injection without replacing the cap.** If the NovoFine disposable needle is not  
470 removed, some liquid may leak out of the PenFill cartridge. This may cause a  
471 change in the strength of suspension insulins (white and cloudy) such as Novolin  
472 N or Novolin 70/30.

473

474 For information on how to throw away needle containers properly, contact your  
475 local trash company.

476 24

477 **SECTION 6 (cont.)**

478

479 **Replace the pen cap:**


480

481 4. After you remove the disposable needle, hold the pen cap so that the clip  
482 is lined up with the dose indicator window.

483

484 5. **Gently slide** the pen cap onto the barrel.

485

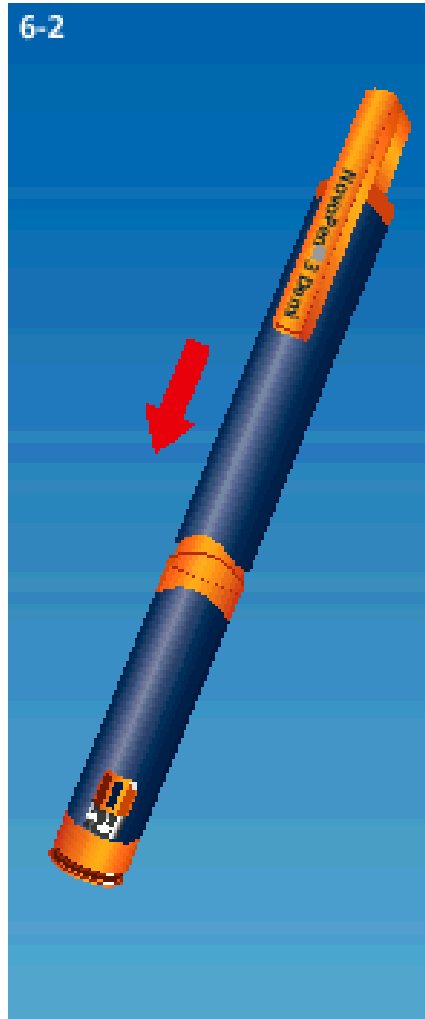

Need Help?  
Call 1-800-727-6500

486  
487  
488  
489

490  
491  
492  
493  
494  
495  
496  
497  
498  
499  
500  
501  
502  
503  
504  
505  
506  
507  
508  
509

## SECTION 7      Removing the PenFill 3 mL Cartridge

You will need to remove the PenFill cartridge for the following reasons:

- ~~When t~~he PenFill cartridge is empty.
- **If you use a suspension insulin such as Novolin N or Novolin 70/30:**

When you see the rear rubber stopper in the inspection window, then you do not have enough insulin left in the PenFill cartridge for proper mixing.

### Remove the barrel:

1. Remove the pen cap.
2. Hold the NovoPen 3 Demi with the dose indicator window at the top.
3. Unscrew the barrel from the cartridge holder.



510  
511  
512

513 **SECTION 7 (cont.)**

514

515 **Remove the PenFill 3 mL cartridge:**

516

517 4. Tip the cartridge holder. The PenFill cartridge will drop out.

518

519 5. Press the push button all the way in until zero (0) appears in the window.


520

521 6. Turn the end of the reset mechanism in a clockwise direction until the  
522 piston rod is no longer sticking out (refer to figure 1-4 on page 7).

523

524 7. To insert a new PenFill cartridge, please refer to Section 2.

525

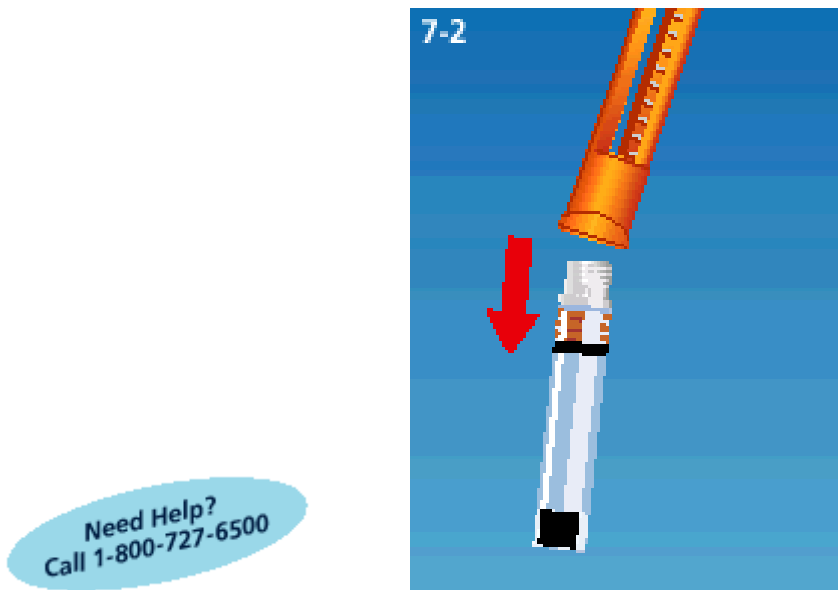

526

527

528 **If the reset mechanism locks, it is usually due to improper technique. Gently turn**  
529 **the mechanism side to side until it unlocks and then call our toll free number (1-**  
530 **800-727-6500) so that we may go over your technique with you.**

531

532



533

## **FUNCTION CHECK**

534

535

You should regularly check the functioning of your NovoPen 3 Demi, (for example, once a month or before starting a new box of PenFill cartridges). The function check is done by delivering 20 units of insulin into the outer needle cap.

537

538

You will not be injecting insulin into your body.

539

540

Always check the functioning of the NovoPen 3 Demi if you suspect it has been damaged or if you are uncertain that it is delivering the correct dose.

541

542

543

Do not use NovoPen 3 Demi unless you are sure that it is working properly.

544

545

### **To perform the function check:**

546

547

1. Attach a NovoFine disposable needle(see pages 12-15).

548

549

2. Do an air shot (see pages 16-19).

550

551

28

552

553  
554  
555  
556  
557  
558  
559  
560

**FUNCTION CHECK (cont.)**

3. **Do not replace the inner needle cap.** Place the outer needle cap securely over the exposed NovoFine needle.



561  
562  
563  
564  
565  
566

**Expel 20 units of insulin into the outer needle cap:**

4. Turn the dial-a-dose selector so the dose indicator window shows 20.



Need Help?  
Call 1-800-727-6500


567

568  
569

570 **FUNCTION CHECK (cont.)**

571  
572  
573  
574  
575  
576  
577  
578  
579  
580  
581  
582  
583  
584  
585

5. Hold the NovoPen 3 Demi so the NovoFine disposable needle is pointing down.
6. Slowly press the push button **as far as it will go**.
7. Check the dose indicator window to see if it shows zero (0). If it does not show zero (0), there is not enough insulin in the cartridge to do a function check. Insert a new PenFill cartridge (see pages 8-11) and repeat the function check. If there is enough insulin in the cartridge but the dose indicator window does not show zero, repeat the FUNCTION CHECK. If you do not see zero after repeating the above steps, do not use your NovoPen 3 Demi. Contact Novo Nordisk Pharmaceuticals, Inc. at our toll free number (1-800-727-6500).

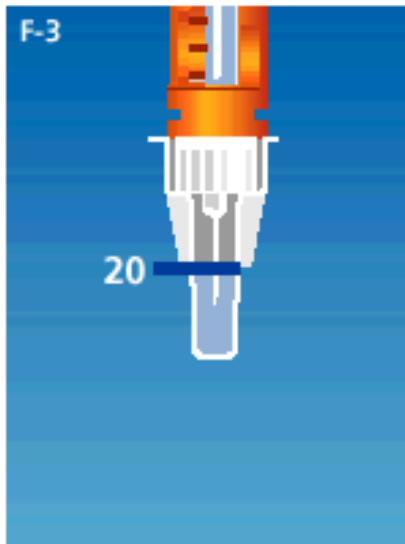

586  
587  
588  
589  
590  
591  
592  
593  
594  
595  
596  
597  
598  
599  
600

The insulin should fill the bottom part of the outer needle cap. This indicates the device is functioning properly.

If the insulin **does not fill or overfills** this part of the cap, review the function check procedure. Then repeat the function check with a new NovoFine disposable needle and outer needle cap.

If the second function check also shows under- or over-filling, do not use your NovoPen 3 Demi.

**DO NOT try to repair a NovoPen 3 Demi that you think is not working properly.**

See Warranty section for further information.



602

603

## STORAGE

604

605

### Guidelines for storing the NovoPen 3 Demi and PenFill 3 mL cartridges:

606

607

- PenFill cartridges should be stored in a cool place, such as in a refrigerator, but not in ~~the~~a freezer.

608

609

610

- After the first use of PenFill cartridge in the NovoPen 3 Demi, the NovoPen 3 Demi (with the PenFill cartridge inside) can be kept at room temperature below 86°F (30°C) for the amount of time-days specified listed in the PenFill Information for the Patient leaflet for the type of insulin you are using.

611

612

613

614

615

616

- **Do not store** the NovoPen 3 Demi (with the PenFill cartridge inside) in a refrigerator or areas where there may be extreme temperatures or moisture, such as in your car.

617

618

619

620

- **The expiration date printed on the cartridge is for unused cartridges under refrigeration. Never use the cartridge after the expiration date on the cartridge or its box.**

621

622

623

624

625

626

- Store the NovoPen 3 Demi **without** the NovoFine needle attached and **with** the pen cap in position.

627

628

629

- For information on storing PenFill cartridges, see the package leaflet that comes in the PenFill cartridge box.

630

631

632

633

634 **MAINTENANCE**

635

636 **Guidelines for maintaining the NovoPen 3 Demi.**

637

638 **Be sure to:**

639

640 1. Clean it by wiping with a soft cloth moistened with alcohol.

641

642 2. Protect it from dust, dirt, and moisture when not in its case.

643

644

645 **Make certain you:**

646

647 1. **Do not** soak it in alcohol, do not wash it in soap and water, or do not  
648 lubricate it, since this may cause damage.

649

650 2. **Do not** expose it to excessive pressure or blows.

651

652 3. **Do not** drop it.

653

654 32

655 **IMPORTANT THINGS TO KNOW**

656

657

- The NovoPen 3 Demi is not recommended for the blind or visually impaired, without the assistance of a sighted individual trained to use it.

658

659

660

- If you use more than one type of insulin (such as Novolin R, Novolin N, or Novolin 70/30, or NovoLog), use a separate insulin delivery device for each type of insulin.

661

662

663

664

- Use only a new PenFill 3 mL cartridge when loading the NovoPen 3 Demi. Never load the NovoPen 3 Demi with a partially filled PenFill cartridge.

665

666

667

- Always keep a spare insulin delivery system available, in case your NovoPen 3 Demi is lost or damaged.

668

669

670

- Keep the NovoPen 3 Demi, PenFill cartridges, and NovoFine needles out of the reach of children. The American Diabetes Association recommends that insulin should be self-administered. The proper age for initiating this should be assessed by the adult caregiver.

671

672

673

674

675

- Keep the NovoPen 3 Demi away from areas where temperatures may get too hot or too cold such as a car or refrigerator.

676

677

678

- The NovoPen 3 Demi is designed for use with PenFill 3 mL insulin cartridges and NovoFine single-use disposable needles.

679

680

681

Novo Nordisk is not responsible for any consequences arising from the use of the NovoPen 3 Demi with products other than PenFill 3 mL insulin cartridges and NovoFine single-use disposable needles.

682

683

684

685



686  
687  
688  
689  
690  
691  
692  
693  
694  
695  
696  
697  
698  
699  
700  
701  
702  
703  
704  
705  
706  
707  
708  
709  
710  
711  
712  
713  
714  
715  
716  
717  
718  
719

**IMPORTANT NOTES**

**The following is a review of some important information about the use and care of your NovoPen 3 Demi.**

**Before each injection, be certain:**

1. The NovoPen 3 Demi contains the correct insulin cartridge (such as Novolin R, Novolin N, Novolin 70/30, or NovoLog), if you use more than one type of insulin.
2. The PenFill cartridge contains enough insulin for mixing, if you use a suspension insulin (white and cloudy) such as Novolin N or Novolin 70/30.
3. To do an air shot with the NovoFine needle pointing up before each injection.

**Be sure to:**

1. Check the dose indicator window after each injection to make sure you have received your full dose (see page 23, Section 5).
2. Remove the NovoFine needle immediately after each injection without replacing the cap.
3. Select your dose only by using the number in the dose indicator window.
4. Perform the function check regularly or if you think your NovoPen 3 Demi is not working properly.

720 **IMPORTANT NOTES (cont.)**

721

722 **Make certain you:**

723

724 1. **DO NOT** place a NovoFine needle on the NovoPen 3 Demi until you are  
725 ready to do an air shot and give an injection or do a function check.

726 Remove the needle immediately after each injection without recapping the  
727 needle. If the NovoFine needle is not removed, some liquid may leak out  
728 of the PenFill cartridge. This may cause a change in the strength of  
729 suspension insulin (white and cloudy) such as Novolin N or Novolin  
730 70/30.

731

732 2. **DO NOT** use the clicking sound to set your insulin dose.

733

734 3. **DO NOT** try to refill a PenFill cartridge.

735

736 4. **DO NOT** share the same PenFill cartridge with anyone else even if you  
737 attach a new NovoFine needle for each injection. Sharing cartridge can  
738 spread disease. Each PenFill cartridge is for single-person use only.

739

740 Blood glucose levels should be tested frequently to monitor your insulin regimen.

741

742 **Any change in insulin should be made cautiously and only under medical**  
743 **supervision.**

744

745

746  
747  
748  
749  
750  
751  
752  
753  
754  
755  
756  
757  
758  
759  
760  
761  
762  
763  
764  
765  
766  
767  
768  
769  
770  
771  
772  
773  
774  
775  
776  
777  
778  
779  
780  
781  
782  
783  
784  
785  
786  
787

**WHAT TO DO IF...**

**The dose indicator window does not show zero after the injection:**

1. **You did not receive your full dose.**  
Follow the steps on page 23 to get the remaining part of your dose.
2. **Your NovoPen 3 Demi is malfunctioning.**  
Do not use your NovoPen 3 Demi. Contact Novo Nordisk Pharmaceuticals, Inc. at our toll free number (1-800-727-6500).

**No insulin appears when you do the air shot:**

1. **The piston rod is not far enough down the cartridge holder to reach the rear rubber stopper.**  
Repeat the air shot (see pages 16-19).
2. **The NovoFine needle may not be securely attached.**
  - a. Put the plastic outer cap back on the NovoFine needle.
  - b. Turn the plastic outer cap in a clockwise direction to tighten the NovoFine needle.
3. **The NovoFine needle may be blocked.**  
Change the NovoFine needle (see pages 14-15) and do an air shot (see pages 16-19).

**The piston rod is sticking out too far to attach the cartridge holder to the barrel:**

You must screw the piston rod back into the barrel (see page 7). Never try to push it in or you can damage the mechanism.

**The push button will not return to zero or the piston rod will not turn back into the reset mechanism:**

The return mechanism may be locked. This is usually due to improper technique. Gently turn the mechanism side to side until it unlocks and then call our toll free number (1-800-727-6500) so that we may review go over your technique with you.

788 **WARRANTY**

789

790

791

792

793

794

795

796

797

798

799

800

801

802

803

804

805

806

807

808

809

810

811

812

813

814

815

816

817

818

Should your NovoPen® 3 Demi device be defective in materials or workmanship within two (2) years of purchase, Novo Nordisk Pharmaceuticals, Inc. will replace it at no charge if you mail the defective unit along with a description of the problem and the sales receipt or other proof of purchase to:

**Novo Nordisk Pharmaceuticals, Inc.**

**Product Safety**

**100 College Road West**

**Princeton, NJ 08540**

Protected by U.S. Patent Nos. 5,693,027; 5,626,566; 6,126,646 and Des. 347,894 (cartridge) restricted to use with Novo Nordisk insulin cartridges and Novo Nordisk pen needles.

No other warranty is made with respect to NovoPen® 3 Demi. This warranty will be invalid and Novo Nordisk A/S, Novo Nordisk Pharmaceuticals, Inc., Bristol-Myers Squibb Co., Nipro Medical Industries Ltd., and Bang & Olufsen A/S cannot be held responsible in the case of defects or damages arising from:

- The use of the NovoPen® 3 Demi with products other than PenFill 3 mL cartridges and NovoFine single-use disposable needles.
- The use of the NovoPen® 3 Demi not in accordance with the instructions in this booklet.
- Physical damage to the NovoPen® 3 Demi caused by neglect, misuse, unauthorized repair, accident, or other breakage.

819 For assistance or further information, write to:

820

821 **Novo Nordisk Pharmaceuticals, Inc.**

822 **Customer Relations**

823 **100 College Road West**

824 **Princeton, NJ 08540**

825

826 **Or call: 1-800-727-6500**

827

828

829 Novo Nordisk®, NovoPen®, Novolin®, NovoLog®, PenFill® and NovoFine® are  
830 registered trademarks of Novo Nordisk A/S

831

832 © 2002 Novo Nordisk A/S

833

834 ***Novo Nordisk Pharmaceuticals, Inc.***

835 Princeton, NJ 08540

836

837 <http://www.novonordisk-us.com>

838

839 8-4241-31-002-1


840

841

1 **NovoLog<sup>®</sup>**  
2 **Insulin aspart (rDNA origin) Injection**

3  
4  
5 **DESCRIPTION**

6 NovoLog<sup>®</sup> (insulin aspart [rDNA origin] injection) is a human insulin analog that is a rapid-  
7 acting, parenteral blood glucose-lowering agent. NovoLog is homologous with regular human  
8 insulin with the exception of a single substitution of the amino acid proline by aspartic acid in  
9 position B28, and is produced by recombinant DNA technology utilizing *Saccharomyces*  
10 *cerevisiae* (baker's yeast) as the production organism. Insulin aspart has the empirical formula  
11 C<sub>256</sub>H<sub>381</sub>N<sub>65</sub>O<sub>79</sub>S<sub>6</sub> and a molecular weight of 5825.8.

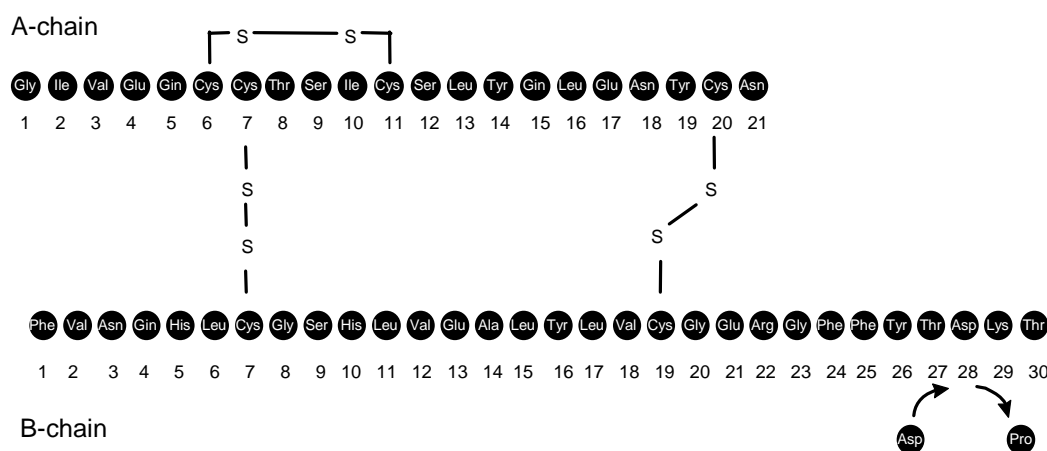

13  
14 Figure 1. Structural formula of insulin aspart.

15  
16 NovoLog is a sterile, aqueous, clear, and colorless solution, that contains insulin aspart (B28  
17 asp regular human insulin analog) 100 Units/mL, glycerin 16 mg/mL, phenol 1.50 mg/mL,  
18 metacresol 1.72 mg/mL, zinc 19.6 µg/mL, disodium hydrogen phosphate dihydrate 1.25  
19 mg/mL, and sodium chloride 0.58 mg/mL. NovoLog has a pH of 7.2-7.6. Hydrochloric acid  
20 10% and/or sodium hydroxide 10% may be added to adjust pH.

21  
22 **CLINICAL PHARMACOLOGY**

23 **Mechanism of Action**

24 The primary activity of NovoLog is the regulation of glucose metabolism. Insulins, including  
25 NovoLog, bind to the insulin receptors on muscle and fat cells and lower blood glucose by  
26 facilitating the cellular uptake of glucose and simultaneously inhibiting the output of glucose  
27 from the liver.

28  
29 In standard biological assays in mice and rabbits, one unit of NovoLog has the same glucose-  
30 lowering effect as one unit of regular human insulin. In humans, the effect of NovoLog is  
31 more rapid in onset and of shorter duration, compared to regular human insulin, due to its  
32 faster absorption after subcutaneous injection (see Figure 2 and Figure 3).


34 **Pharmacokinetics**

35 The single substitution of the amino acid proline with aspartic acid at position B28 in  
36 NovoLog reduces the molecule's tendency to form hexamers as observed with regular human  
37 insulin. NovoLog is therefore more rapidly absorbed after subcutaneous injection compared to  
38 regular human insulin.

39

40 *Bioavailability and Absorption* - NovoLog has a faster absorption, a faster onset of action, and  
41 a shorter duration of action than regular human insulin after subcutaneous injection (see Figure  
42 2 and Figure 3). The relative bioavailability of NovoLog compared to regular human insulin  
43 indicates that the two insulins are absorbed to a similar extent.

44

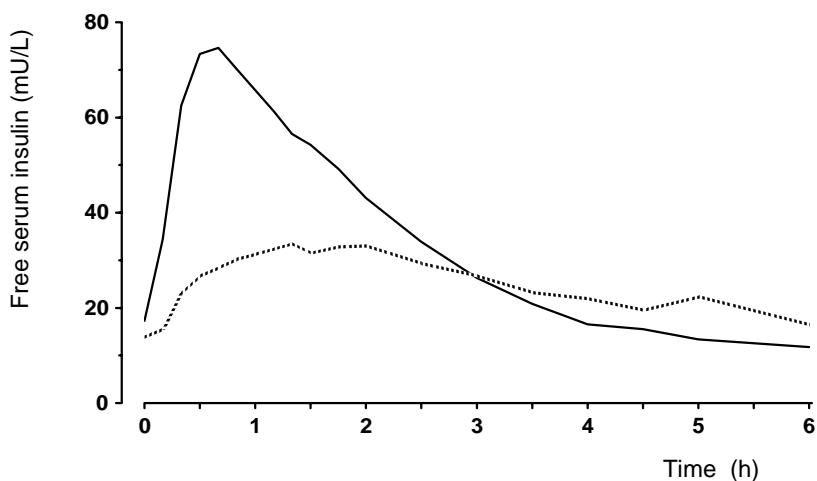

45

46

47 Figure 2. Serial mean serum free insulin concentration collected up to 6 hours following a  
48 single pre-meal dose of NovoLog (solid curve) or regular human insulin (hatched curve)  
49 injected immediately before a meal in 22 patients with Type 1 diabetes.

50

51 In studies in healthy volunteers (total n=107) and patients with Type 1 diabetes (total n=40),  
52 NovoLog consistently reached peak serum concentrations approximately twice as fast as  
53 regular human insulin. The median time to maximum concentration in these trials was 40 to  
54 50 minutes for NovoLog versus 80 to 120 minutes for regular human insulin. In a clinical trial  
55 in patients with Type 1 diabetes, NovoLog and regular human insulin, both administered  
56 subcutaneously at a dose of 0.15 U/kg body weight, reached mean maximum concentrations of  
57 82.1 and 35.9 mU/L, respectively. Pharmacokinetic/pharmacodynamic characteristics of  
58 insulin aspart have not been established in patients with Type 2 diabetes.

59 The intra-individual variability in time to maximum serum insulin concentration for healthy  
60 male volunteers was significantly less for NovoLog than for regular human insulin. The  
61 clinical significance of this observation has not been established.

62 In a clinical study in healthy non-obese subjects, the pharmacokinetic differences between  
63 NovoLog and regular human insulin described above, were observed independent of the  
64 injection site (abdomen, thigh, or upper arm).

65

66 *Distribution and Elimination* - NovoLog has a low binding to plasma proteins, 0-9%, similar  
67 to regular human insulin. After subcutaneous administration in normal male volunteers  
68 (n=24), NovoLog was more rapidly eliminated than regular human insulin with an average  
69 apparent half-life of 81 minutes compared to 141 minutes for regular human insulin.


70

### 71 **Pharmacodynamics**

72 Studies in normal volunteers and patients with diabetes demonstrated that NovoLog has a  
73 more rapid onset of action than regular human insulin.

74 In a 6-hour study in patients with Type 1 diabetes (n=22), the maximum glucose-lowering  
75 effect of NovoLog occurred between 1 and 3 hours after subcutaneous injection (see Figure 3).  
76 The duration of action for NovoLog is 3 to 5 hours compared to 5 to 8 hours for regular human  
77 insulin. The time course of action of insulin and insulin analogs such as NovoLog may vary  
78 considerably in different individuals or within the same individual. The parameters of  
79 NovoLog activity (time of onset, peak time and duration) as designated in Figure 3 should be  
80 considered only as general guidelines. The rate of insulin absorption and consequently the  
81 onset of activity is known to be affected by the site of injection, exercise, and other variables  
82 (see PRECAUTIONS, General).

83

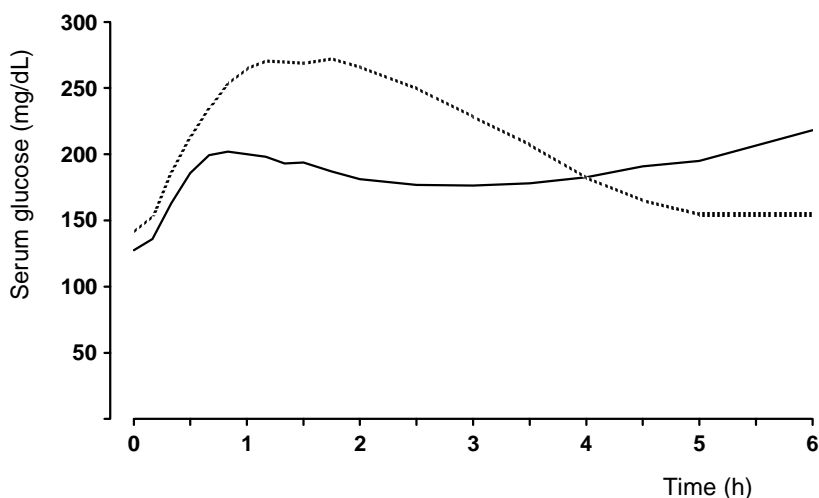

84

85

86 Figure 3. Serial mean serum glucose collected up to 6 hours following a single pre-meal dose  
87 of NovoLog (solid curve) or regular human insulin (hatched curve) injected immediately  
88 before a meal in 22 patients with Type 1 diabetes.

89

### 90 **Special Populations**

91 *Children and Adolescents* - The pharmacokinetic and pharmacodynamic properties of  
92 NovoLog and regular human insulin were evaluated in a single dose study in 18 children (6-12  
93 years, n=9) and adolescents (13-17 years [Tanner grade  $\geq 2$ ], n=9) with Type 1 diabetes. The  
94 relative differences in pharmacokinetics and pharmacodynamics in children and adolescents  
95 with Type 1 diabetes between NovoLog and regular human insulin were similar to those in  
96 healthy adult subjects and adults with Type 1 diabetes.

97



98 *Geriatrics* - The effect of age on the pharmacokinetics and pharmacodynamics of NovoLog  
99 has not been studied.

100

101 *Gender* - In healthy volunteers, no difference in insulin aspart levels was seen between men  
102 and women when body weight differences were taken into account. There was no significant  
103 difference in efficacy noted (as assessed by HbA1c) between genders in a trial in patients with  
104 Type 1 diabetes.

105

106 *Obesity* - The effect of obesity and/or subcutaneous fat thickness on the pharmacokinetics and  
107 glucodynamics of NovoLog has not been studied.

108

109 *Ethnic Origin* - The effect of ethnic origin on the pharmacokinetics of NovoLog has not been  
110 studied.

111

112 *Renal Impairment* - Some studies with human insulin have shown increased circulating levels  
113 of insulin in patients with renal failure. The effect of renal impairment on the pharmacokinetics  
114 of NovoLog has not been studied. Careful glucose monitoring and dose adjustments of  
115 insulin, including NovoLog, may be necessary in patients with renal dysfunction (see  
116 PRECAUTIONS, Renal Impairment).

117

118 *Hepatic Impairment* - Some studies with human insulin have shown increased circulating  
119 levels of insulin in patients with liver failure. The effect of hepatic impairment on the  
120 pharmacokinetics of NovoLog has not been studied. Careful glucose monitoring and dose  
121 adjustments of insulin, including NovoLog, may be necessary in patients with hepatic  
122 dysfunction (see PRECAUTIONS, Hepatic Impairment).

123

124 *Pregnancy* - The effect of pregnancy on the pharmacokinetics and glucodynamics of  
125 Novolog has not been studied (see PRECAUTIONS, Pregnancy).

126

127 *Smoking* - The effect of smoking on the pharmacokinetics/pharmacodynamics of NovoLog has  
128 not been studied.

129

### 130 **CLINICAL STUDIES**

131 To evaluate the safety and efficacy of NovoLog in patients with Type 1 diabetes, two  
132 six-month, open-label, active-control (NovoLog<sup>®</sup> vs. Novolin<sup>®</sup> R) studies were conducted (see  
133 Table 1). NovoLog was administered by subcutaneous injection immediately prior to meals  
134 and regular human insulin was administered by subcutaneous injection 30 minutes before  
135 meals. NPH insulin was administered as the basal insulin in either single or divided daily  
136 doses. Glycemic control (as measured by HbA1c), the rates of hypoglycemia (as determined  
137 from the number of events requiring intervention from a third party), and the incidence of  
138 ketosis were clinically comparable for the two treatment regimens. The mean total daily doses  
139 of insulin were greater (1-3 U/day) in the NovoLog-treated patients compared to patients who  
140 received regular human insulin. This difference was primarily due to basal insulin  
141 requirements. To achieve the stated levels of glycemic control, some patients required more

142 than three doses of meal-related insulin and/or more than one dose of basal insulin (see Table  
143 1). No serum glucose measurements were obtained in these studies.

144  
145 To evaluate the safety and efficacy of NovoLog in patients with Type 2 diabetes, one six-  
146 month, open-label, active-control (NovoLog<sup>®</sup> vs. Novolin<sup>®</sup> R) study was conducted (see Table  
147 1). NovoLog was administered by subcutaneous injection immediately prior to meals and  
148 regular human insulin was administered by subcutaneous injection 30 minutes before meals.  
149 NPH insulin was administered as the basal insulin in either single or divided daily doses.  
150 Glycemic control (as measured by HbA1c) and the rates of hypoglycemia (as determined from  
151 the number of events requiring intervention from a third party) were clinically comparable for  
152 the two treatment regimens. The mean total daily dose of insulin was greater (2 U/day) in the  
153 NovoLog-treated patients compared to patients who received regular human insulin. This  
154 difference was primarily due to basal insulin requirements. To achieve the stated levels of  
155 glycemic control, some patients required more than three doses of meal-related insulin and/or  
156 more than one dose of basal insulin (see Table 1).

157  
158 Table 1. Results of two six-month, active-control, open-label trials in patients with Type 1  
159 diabetes (Studies A and B) and one six-month, active-control, open-label trial in patients with  
160 Type 2 diabetes (Study C).

161

Study	Treatment (n)	Mean HbA1c (%)		Hypoglycemia <sup>1</sup> (events / month / patient)	% of Patients Using Various Numbers of Insulin Injections / Day <sup>2</sup>				
		Baseline	Month 6		Rapid-acting			Basal	
					1 - 2	3	4 - 5	1	2
A	NovoLog (n=694)	8.0	7.9	0.06	3	75	22	54	46
	Novolin R (n=346)	8.0	8.0	0.06	6	75	19	63	37
B	NovoLog (n=573)	7.9	7.8	0.08	4	90	6	94	6
	Novolin R (n=272)	8.0	7.9	0.06	4	91	4	93	7
C	NovoLog (n=90)	8.1	7.7	0.02	4	93	4	97	4
	Novolin R (n=86)	7.8	7.8	0.01	2	93	5	93	7

162 <sup>1</sup> Events requiring intervention from a third party during the last three months of treatment

163 <sup>2</sup> Percentages are rounded to the nearest whole number

164

165 To evaluate the use of NovoLog by subcutaneous infusion with an external pump, two open-  
166 label, parallel design studies (6 weeks [n=29] and 16 weeks [n=118]) compared NovoLog  
167 versus Velosulin (buffered regular human insulin) in patients with Type 1 diabetes. Glycemic  
168 control (as measured by HbA1c) and rates of hypoglycemia were comparable. Patients with  
169 Type 2 diabetes were also studied in an open-label, parallel design trial (16 weeks [n=127])  
170 using NovoLog by subcutaneous infusion compared to pre-prandial injection (in conjunction  
171 with basal NPH injections). Reductions in HbA1c and rates of hypoglycemia were comparable.  
172 (See INDICATIONS AND USAGE, WARNINGS, PRECAUTIONS, Mixing of Insulins,  
173 Information for Patients, DOSAGE AND ADMINISTRATION, and RECOMMENDED  
174 STORAGE.)

175

176 **INDICATIONS AND USAGE**

177 NovoLog is indicated for the treatment of adult patients with diabetes mellitus, for the control  
178 of hyperglycemia. Because NovoLog has a more rapid onset and a shorter duration of activity  
179 than human regular insulin, NovoLog given by injection should normally be used in regimens  
180 with an intermediate or long-acting insulin. NovoLog may also be infused subcutaneously by  
181 external insulin pumps. (See WARNINGS, PRECAUTIONS [especially Usage in Pumps],  
182 Information for Patients [especially For Patients Using Pumps], Mixing of Insulins, DOSAGE  
183 AND ADMINISTRATION, RECOMMENDED STORAGE.)

184  
185 **CONTRAINDICATIONS**

186 NovoLog is contraindicated during episodes of hypoglycemia and in patients hypersensitive to  
187 NovoLog or one of its excipients.

188  
189 **WARNINGS**

190 **NovoLog differs from regular human insulin by a more rapid onset and a shorter**  
191 **duration of activity. Because of the fast onset of action, the injection of NovoLog should**  
192 **immediately be followed by a meal. Because of the short duration of action of NovoLog,**  
193 **patients with diabetes also require a longer-acting insulin to maintain adequate glucose**  
194 **control. Glucose monitoring is recommended for all patients with diabetes and is**  
195 **particularly important for patients using external pump infusion therapy.**

196  
197 **Hypoglycemia is the most common adverse effect of insulin therapy, including NovoLog.**  
198 **As with all insulins, the timing of hypoglycemia may differ among various insulin**  
199 **formulations.**

200  
201 **Any change of insulin dose should be made cautiously and only under medical**  
202 **supervision. Changes in insulin strength, manufacturer, type (e.g., regular, NPH,**  
203 **analog), species (animal, human), or method of manufacture (rDNA versus animal-**  
204 **source insulin) may result in the need for a change in dosage.**

205  
206 **Insulin Pumps: When used in an external insulin pump for subcutaneous infusion,**  
207 **NovoLog should not be diluted or mixed with any other insulin. Physicians and patients**  
208 **should carefully evaluate information on pump use in the NovoLog physician and patient**  
209 **package inserts and in the pump manufacturer's manual (e.g. NovoLog-specific**  
210 **information should be followed for in-use time, frequency of changing infusion sets, or**  
211 **other details specific to NovoLog usage, because NovoLog-specific information may**  
212 **differ from general pump manual instructions). Pump or infusion set malfunctions or**  
213 **insulin degradation can lead to hyperglycemia and ketosis in a short time because of the**  
214 **small subcutaneous depot of insulin. This is especially pertinent for rapid-acting insulin**  
215 **analogs that are more rapidly absorbed through skin and have shorter duration of**  
216 **action. These differences may be particularly relevant when patients are switched from**  
217 **multiple injection therapy or infusion with buffered regular insulin. Prompt**  
218 **identification and correction of the cause of hyperglycemia or ketosis is necessary.**  
219 **Interim therapy with subcutaneous injection may be required. (See PRECAUTIONS,**

220 **Mixing of Insulins, Information for Patients, DOSAGE AND ADMINISTRATION, and**  
221 **RECOMMENDED STORAGE.)**

222

223 **PRECAUTIONS**

224 **General**

225 Hypoglycemia and hypokalemia are among the potential clinical adverse effects associated  
226 with the use of all insulins. Because of differences in the action of NovoLog and other  
227 insulins, care should be taken in patients in whom such potential side effects might be  
228 clinically relevant (e.g., patients who are fasting, have autonomic neuropathy, or are using  
229 potassium-lowering drugs or patients taking drugs sensitive to serum potassium level).

230 Lipodystrophy and hypersensitivity are among other potential clinical adverse effects  
231 associated with the use of all insulins.

232 As with all insulin preparations, the time course of NovoLog action may vary in different  
233 individuals or at different times in the same individual and is dependent on site of injection,  
234 blood supply, temperature, and physical activity.

235 Adjustment of dosage of any insulin may be necessary if patients change their physical activity  
236 or their usual meal plan. Insulin requirements may be altered during illness, emotional  
237 disturbances, or other stresses.

238

239 *Hypoglycemia* - As with all insulin preparations, hypoglycemic reactions may be associated  
240 with the administration of NovoLog. Rapid changes in serum glucose levels may induce  
241 symptoms of hypoglycemia in persons with diabetes, regardless of the glucose value. Early  
242 warning symptoms of hypoglycemia may be different or less pronounced under certain  
243 conditions, such as long duration of diabetes, diabetic nerve disease, use of medications such  
244 as beta-blockers, or intensified diabetes control (see PRECAUTIONS, Drug Interactions).  
245 Such situations may result in severe hypoglycemia (and, possibly, loss of consciousness) prior  
246 to patients' awareness of hypoglycemia.

247

248 *Renal Impairment* - Although there are no specific data in patients with diabetes and renal  
249 impairment treated with NovoLog, NovoLog dose requirements may be reduced in the  
250 presence of renal impairment, similar to observations with other insulins (see CLINICAL  
251 PHARMACOLOGY, Pharmacokinetics).

252

253 *Hepatic Impairment* - Although there are no specific data in patients with diabetes and  
254 hepatic disease treated with NovoLog, NovoLog dose requirements may be reduced in the  
255 presence of impaired hepatic function, similar to observations found with other insulins (see  
256 CLINICAL PHARMACOLOGY, Pharmacokinetics).

257

258 *Allergy - Local Allergy* - As with other insulin therapy, patients may experience redness,  
259 swelling, or itching at the site of injection. These minor reactions usually resolve in a few days  
260 to a few weeks, but in some occasions, may require discontinuation of NovoLog. In some  
261 instances, these reactions may be related to factors other than insulin, such as irritants in a skin  
262 cleansing agent or poor injection technique.

263 *Systemic Allergy* - Less common, but potentially more serious, is generalized allergy to insulin,  
264 which may cause rash (including pruritus) over the whole body, shortness of breath, wheezing,

265 reduction in blood pressure, rapid pulse, or sweating. Severe cases of generalized allergy,  
266 including anaphylactic reaction, may be life threatening.

267 Localized reactions and generalized myalgias have been reported with the use of cresol as an  
268 injectable excipient.

269 In controlled clinical trials using injection therapy, allergic reactions were reported in 3 of 735  
270 patients (0.4%) who received regular human insulin and 10 of 1394 patients (0.7%) who  
271 received NovoLog. During these and other trials, 3 of 2341 patients treated with NovoLog  
272 were discontinued due to allergic reactions.

273

274 *Antibody Production* - Insulin antibodies may develop during treatment with insulin. In large  
275 clinical trials, levels of antibodies that cross react with human insulin and insulin aspart were  
276 higher in patients treated with NovoLog compared to regular human insulin. The clinical  
277 significance of these antibodies is uncertain.

278

#### 279 *Pregnancy and Lactation*

280 Female patients should be advised to tell their physician if they intend to become, or if they  
281 become pregnant. Information is not available on the use of NovoLog during pregnancy or  
282 lactation.

283

#### 284 *Usage in Pumps*

285 NovoLog is recommended for use in Disetronic H-TRON<sup>®</sup> plus V100 with Disetronic 3.15  
286 plastic cartridges and Classic or Tender infusion sets; MiniMed Models 505, 506, or 507 with  
287 MiniMed 3 mL syringes and Polyfin<sup>®</sup> or Sof-set<sup>®</sup> infusion sets.

288

289 In-vitro studies have shown that pump malfunction, loss of cresol, and insulin degradation,  
290 may occur with the use of NovoLog for more than two days at 37°C (98.6°F) in infusion sets  
291 and reservoirs. NovoLog in clinical use should not be exposed to temperatures greater than  
292 37°C (98.6°F). **NovoLog should not be mixed with other insulins or with a diluent when it  
293 is used in the pump.** (See WARNINGS, PRECAUTIONS, Mixing of Insulins, Information  
294 for Patients, DOSAGE AND ADMINISTRATION, and RECOMMENDED STORAGE.)

295

296

### 297 **Information for Patients**

298

#### 299 *For all patients:*

300 Patients should be informed about potential risks and advantages of NovoLog therapy  
301 including the possible side effects. Patients should also be offered continued education and  
302 advice on insulin therapies, injection technique, life-style management, regular glucose  
303 monitoring, periodic glycosylated hemoglobin testing, recognition and management of hypo-  
304 and hyperglycemia, adherence to meal planning, complications of insulin therapy, timing of  
305 dose, instruction in the use of injection or subcutaneous infusion devices, and proper storage of  
306 insulin. Patients should be informed that frequent, patient-performed blood glucose  
307 measurements are needed to achieve optimal glycemic control and avoid both hyper- and  
308 hypoglycemia.

309

310 Female patients should be advised to tell their physician if they intend to become, or if they  
311 become pregnant. Information is not available on the use of NovoLog during pregnancy or  
312 lactation (see PRECAUTIONS, Pregnancy).

313

#### 314 *For patients using pumps*

315 Patients using external pump infusion therapy should be trained in intensive insulin therapy  
316 with multiple injections and in the function of their pump and pump accessories. NovoLog is  
317 recommended for use with Disetronic H-TRON plus V100 with Disetronic 3.15 plastic  
318 cartridges and Classic or Tender infusion sets; MiniMed Models 505, 506, and 507 with  
319 MiniMed 3 mL syringes and Polyfin or Sof-set infusion sets. The use of NovoLog in quick-  
320 release infusion sets and cartridge adapters has not been assessed.

321

322 **To avoid insulin degradation, infusion set occlusion, and loss of the preservative (cresol),**  
323 **the infusion sets (reservoir syringe, tubing, and catheter) and the NovoLog in the**  
324 **reservoir should be replaced, and a new infusion site selected every 48 hours or less.**  
325 **Insulin exposed to temperatures higher than 37°C (98.6°F) should be discarded.** The  
326 temperature of the insulin may exceed ambient temperature when the pump housing, cover,  
327 tubing, or sport case is exposed to sunlight or radiant heat. Infusion sites that are erythematous,  
328 pruritic, or thickened should be reported to medical personnel, and a new site selected because  
329 continued infusion may increase the skin reaction and/or alter the absorption of NovoLog.

330

331 Pump or infusion set malfunctions or insulin degradation can lead to hyperglycemia and  
332 ketosis in a short time because of the small subcutaneous depot of insulin. This is especially  
333 pertinent for rapid-acting insulin analogs that are more rapidly absorbed through skin and have  
334 shorter duration of action. These differences are particularly relevant when patients are  
335 switched from infused buffered regular insulin or multiple injection therapy. Prompt  
336 identification and correction of the cause of hyperglycemia or ketosis is necessary. Problems  
337 include pump malfunction, infusion set occlusion, leakage, disconnection or kinking, and  
338 degraded insulin. Less commonly, hypoglycemia from pump malfunction may occur. If these  
339 problems cannot be promptly corrected, patients should resume therapy with subcutaneous  
340 insulin injection and contact their physician. (See WARNINGS, PRECAUTIONS, Mixing of  
341 Insulins, DOSAGE AND ADMINISTRATION, and RECOMMENDED STORAGE.)

342

#### 343 **Laboratory Tests**

344 As with all insulin therapy, the therapeutic response to NovoLog should be monitored by  
345 periodic blood glucose tests. Periodic measurement of glycosylated hemoglobin is  
346 recommended for the monitoring of long-term glycemic control.

347

#### 348 **Drug Interactions**

349 A number of substances affect glucose metabolism and may require insulin dose adjustment  
350 and particularly close monitoring.

- 351 • The following are examples of substances that may increase the blood-glucose-lowering  
352 effect and susceptibility to hypoglycemia: oral antidiabetic products, ACE inhibitors,  
353 disopyramide, fibrates, fluoxetine, monoamine oxidase (MAO) inhibitors, propoxyphene,  
354 salicylates, somatostatin analog (e.g., octreotide), sulfonamide antibiotics.

- 355 • The following are examples of substances that may reduce the blood-glucose-lowering  
356 effect: corticosteroids, niacin, danazol, diuretics, sympathomimetic agents (e.g.,  
357 epinephrine, salbutamol, terbutaline), isoniazid, phenothiazine derivatives, somatropin,  
358 thyroid hormones, estrogens, progestogens (e.g., in oral contraceptives).
- 359 • Beta-blockers, clonidine, lithium salts, and alcohol may either potentiate or weaken the  
360 blood-glucose-lowering effect of insulin. Pentamidine may cause hypoglycemia, which  
361 may sometimes be followed by hyperglycemia.
- 362 • In addition, under the influence of sympatholytic medicinal products such as beta-blockers,  
363 clonidine, guanethidine, and reserpine, the signs of hypoglycemia may be reduced or  
364 absent (see CLINICAL PHARMACOLOGY).
- 365

### 366 **Mixing of Insulins**

- 367 • A clinical study in healthy male volunteers (n=24) demonstrated that mixing NovoLog  
368 with NPH human insulin immediately before injection produced some attenuation in the  
369 peak concentration of NovoLog, but that the time to peak and the total bioavailability of  
370 NovoLog were not significantly affected. If NovoLog is mixed with NPH human insulin,  
371 NovoLog should be drawn into the syringe first. The injection should be made  
372 immediately after mixing. Because there are no data on the compatibility of NovoLog and  
373 crystalline zinc insulin preparations, NovoLog should not be mixed with these  
374 preparations.
- 375 • The effects of mixing NovoLog with insulins of animal source or insulin preparations  
376 produced by other manufacturers have not been studied (see WARNINGS).
- 377 • Mixtures should not be administered intravenously.
- 378 • When used in external subcutaneous infusion pumps for insulin, NovoLog should not be  
379 mixed with any other insulins or diluent.
- 380

### 381 **Carcinogenicity, Mutagenicity, Impairment of Fertility**

382 Standard 2-year carcinogenicity studies in animals have not been performed to evaluate the  
383 carcinogenic potential of NovoLog. In 52-week studies, Sprague-Dawley rats were dosed  
384 subcutaneously with NovoLog at 10, 50, and 200 U/kg/day (approximately 2, 8, and 32 times  
385 the human subcutaneous dose of 1.0 U/kg/day, based on U/body surface area, respectively). At  
386 a dose of 200 U/kg/day, NovoLog increased the incidence of mammary gland tumors in  
387 females when compared to untreated controls. The incidence of mammary tumors for  
388 NovoLog was not significantly different than for regular human insulin. The relevance of  
389 these findings to humans is not known. NovoLog was not genotoxic in the following tests:  
390 Ames test, mouse lymphoma cell forward gene mutation test, human peripheral blood  
391 lymphocyte chromosome aberration test, in vivo micronucleus test in mice, and in *ex vivo*  
392 UDS test in rat liver hepatocytes. In fertility studies in male and female rats, at subcutaneous  
393 doses up to 200 U/kg/day (approximately 32 times the human subcutaneous dose, based on  
394 U/body surface area), no direct adverse effects on male and female fertility, or general  
395 reproductive performance of animals was observed.

396

### 397 **Pregnancy - Teratogenic Effects - Pregnancy Category C**

398 There are no adequate well-controlled clinical studies of the use of NovoLog in pregnant  
399 women. NovoLog should be used during pregnancy only if the potential benefit justifies the  
400 potential risk to the fetus.

401

402 It is essential for patients with diabetes or history of gestational diabetes to maintain good  
403 metabolic control before conception and throughout pregnancy. Insulin requirements may  
404 decrease during the first trimester, generally increase during the second and third trimesters,  
405 and rapidly decline after delivery. Careful monitoring of glucose control is essential in such  
406 patients.

407

408 Subcutaneous reproduction and teratology studies have been performed with NovoLog and  
409 regular human insulin in rats and rabbits. In these studies, NovoLog was given to female rats  
410 before mating, during mating, and throughout pregnancy, and to rabbits during organogenesis.  
411 The effects of NovoLog did not differ from those observed with subcutaneous regular human  
412 insulin. NovoLog, like human insulin, caused pre- and post-implantation losses and  
413 visceral/skeletal abnormalities in rats at a dose of 200 U/kg/day (approximately 32 times the  
414 human subcutaneous dose of 1.0 U/kg/day, based on U/body surface area) and in rabbits at a  
415 dose of 10 U/kg/day (approximately three times the human subcutaneous dose of 1.0 U/kg/day,  
416 based on U/body surface area). The effects are probably secondary to maternal hypoglycemia  
417 at high doses. No significant effects were observed in rats at a dose of 50 U/kg/day and rabbits  
418 at a dose of 3 U/kg/day. These doses are approximately 8 times the human subcutaneous dose  
419 of 1.0 U/kg/day for rats and equal to the human subcutaneous dose of 1.0 U/kg/day for rabbits,  
420 based on U/body surface area.

421

#### 422 **Nursing Mothers**

423 It is unknown whether insulin aspart is excreted in human milk. Many drugs, including human  
424 insulin, are excreted in human milk. For this reason, caution should be exercised when  
425 NovoLog is administered to a nursing mother.

426

#### 427 **Pediatric Use**

428 Safety and effectiveness of NovoLog in children have not been studied.

429

#### 430 **Geriatric Use**

431 In the large controlled clinical trials, 36 patients  $\geq$  65 years of age were treated with NovoLog.  
432 No conclusions regarding the safety and efficacy of NovoLog in the elderly patients compared  
433 to younger adults can be reached from this limited data set.

434

#### 435 **ADVERSE REACTIONS**

436 Clinical trials comparing NovoLog with regular human insulin did not demonstrate a  
437 difference in frequency of adverse events between the two treatments.

438 Adverse events commonly associated with human insulin therapy include the following:

439 **Body as Whole** - *Allergic reactions* (see PRECAUTIONS, Allergy).

440 **Skin and Appendages** - *Injection site reaction, lipodystrophy, pruritus, rash* (see  
441 PRECAUTIONS, Allergy; Information for Patients, Usage in Pumps.).

442 **Other** – *Hypoglycemia, Hyperglycemia and ketosis* (see WARNINGS and PRECAUTIONS).



443 In controlled clinical trials, small, but persistent elevations in alkaline phosphatase result were  
444 observed in some patients treated with NovoLog. The clinical significance of this finding is  
445 unknown.

446

#### 447 **OVERDOSAGE**

448 Hypoglycemia may occur as a result of an excess of insulin relative to food intake, energy  
449 expenditure, or both. Mild episodes of hypoglycemia usually can be treated with oral glucose.  
450 Adjustments in drug dosage, meal patterns, or exercise, may be needed. More severe episodes  
451 with coma, seizure, or neurologic impairment may be treated with intramuscular/subcutaneous  
452 glucagon or concentrated intravenous glucose. Sustained carbohydrate intake and observation  
453 may be necessary because hypoglycemia may recur after apparent clinical recovery.

454

#### 455 **DOSAGE AND ADMINISTRATION**

456 NovoLog should generally be given immediately before a meal (start of meal within 5-10  
457 minutes after injection) because of its fast onset of action. The dosage of  
458 NovoLog should be individualized and determined, based on the physician's advice, in  
459 accordance with the needs of the patient. The total daily individual insulin requirement is  
460 usually between 0.5-1.0 units/kg/day. When used in a meal-related subcutaneous injection  
461 treatment regimen, 50-70% of total insulin requirements may be provided by NovoLog and the  
462 remainder provided by an intermediate-acting or long-acting insulin. When used in external  
463 insulin infusion pumps, the initial programming of the pump is based on the total daily insulin  
464 dose of the previous regimen. Although there is significant interpatient variability,  
465 approximately 50% of the total dose is given as meal-related boluses of NovoLog and the  
466 remainder as basal infusion. Because of NovoLog's comparatively rapid onset and short  
467 duration of glucose lowering activity, some patients may require more basal insulin and more  
468 total insulin to prevent pre-meal hyperglycemia when using NovoLog than when using human  
469 regular insulin. Additional basal insulin injections, or higher basal rates in external  
470 subcutaneous infusion pumps may be necessary. **Infusion sets and the insulin in the infusion  
471 sets must be changed every 48 hours or sooner to assure the activity of NovoLog and  
472 proper pump function.** (See WARNINGS, PRECAUTIONS, Information for Patients)

473

474 NovoLog should be administered by subcutaneous injection in the abdominal wall, the thigh,  
475 or the upper arm, or by continuous subcutaneous infusion in the abdominal wall. Injection  
476 sites and infusion sites should be rotated within the same region. As with all insulins, the  
477 duration of action will vary according to the dose, injection site, blood flow, temperature, and  
478 level of physical activity.

479 Parenteral drug products should be inspected visually for particulate matter and discoloration  
480 prior to administration, whenever solution and container permit. Never use any NovoLog if it  
481 has become viscous (thickened) or cloudy; use it only if it is clear and colorless. NovoLog  
482 should not be used after the printed expiration date.

483

#### 484 **HOW SUPPLIED**

485 NovoLog<sup>®</sup> is available in the following package sizes: each presentation containing 100 Units  
486 of insulin aspart per mL (U-100).

487 10 mL vials

NDC 0169-7501-11

488 3 mL PenFill<sup>®</sup> cartridges\* NDC 0169-3303-12  
489

490 \* NovoLog<sup>®</sup> PenFill<sup>®</sup> cartridges are for use with NovoPen<sup>®</sup>3, NovoPen<sup>®</sup>3 Demi, and NovoPen  
491 Junior Insulin Delivery Devices  
492 and NovoFine<sup>®</sup> disposable needles.  
493

494 **RECOMMENDED STORAGE**

495 NovoLog in unopened vials and cartridges should be stored between 2° and 8°C (36° to 46°F).  
496 *Do not freeze. Do not use NovoLog if it has been frozen or exposed to temperatures that*  
497 **exceed 37°C (98.6°F).** After a vial or cartridge has been punctured, it may be kept at  
498 temperatures below 30°C (86°F) for up to 28 days, but should not be exposed to excessive heat  
499 or sunlight. Opened vials may be refrigerated. Cartridges should not be refrigerated after  
500 insertion into the NovoPen 3. Infusion sets (reservoirs, tubing, and catheters) and the NovoLog  
501 in the reservoir should be discarded after no more than 48 hours of use or after exposure to  
502 temperatures that exceed 37°C (98.6°F).  
503

504 Rx only  
505

506 Date of Issue: December 21, 2001  
507 8-XXXX-XX-XXX-X  
508

509 Manufactured For Novo Nordisk Pharmaceuticals Inc., Princeton, New Jersey 08540  
510 [www.novonordisk-us.com](http://www.novonordisk-us.com)

511 Manufactured By Novo Nordisk A/S, 2880 Bagsvaerd, Denmark  
512

513 NovoLog<sup>®</sup>, NovoPen<sup>®</sup> 3, PenFill<sup>®</sup>, Novolin<sup>®</sup> and NovoFine<sup>®</sup> are trademarks of Novo Nordisk  
514 A/S

515 Polyfin<sup>®</sup> and Sofset<sup>®</sup> are trademarks of Medtronic MiniMed, Inc.

516 H-TRON<sup>®</sup> is a trademark of Disetronic Medical Systems, Inc.

1  
2  
3 **Information For The Patient**  
4 **NovoLog<sup>®</sup> (Insulin aspart [rDNA origin] Injection)**  
5 **3 mL PenFill<sup>®</sup> Disposable Cartridge (300 units per cartridge)**  
6 **10 mL Vial (1000 units per vial)**  
7 **100 units/mL (U-100)**

- 8 • What is the most important information I should know about NovoLog?  
9 • For all NovoLog users  
10 • For pump users  
11 • What is NovoLog?  
12 • Who should not use NovoLog?  
13 • What should I know about using insulin?  
14 • What should I know about using NovoLog?  
15 • What should I avoid when using NovoLog?  
16 • What are the possible side effects of NovoLog?  
17 • How should I store NovoLog?  
18 • General advice  
19 • Injection and pump infusion instructions  
20 • How should I inject NovoLog?  
21 • Using Vials  
22 • Using Cartridges  
23 • How should I infuse NovoLog with an external subcutaneous insulin infusion  
24 pump?  
25 • How should I mix insulins?

26  
27 Read this information carefully before you begin treatment. Read the information you  
28 get whenever you get more medicine. There may be new information. This information  
29 does not take the place of talking with your doctor about your medical condition or your  
30 treatment. If you have any questions about NovoLog<sup>®</sup> (NO-voe-log), ask your doctor.  
31 Only your doctor can determine if NovoLog<sup>®</sup> is right for you.

32  
33 **What is the most important information I should know about NovoLog?**

34  
35 *For All NovoLog Users*

- 36 • NovoLog (NO-voe-log) is different from regular human insulin and buffered regular  
37 human insulin (Velosulin). It works faster (rapid onset of action) and will not work as  
38 long (shorter duration of action) as regular human insulin or buffered regular human  
39 insulin (Velosulin).  
40  
41 • Because the onset of action is fast, you should eat a meal 5-10 minutes after a  
42 NovoLog injection or NovoLog bolus infusion dose given by an external pump. (A  
43 bolus is a large dose.) Eating right after the dose will reduce the risk of low blood  
44 sugar (hypoglycemia).  
45

- 46 • The shorter duration of NovoLog's action means that you may need to use an  
47 intermediate or longer-acting insulin (basal insulin) or higher basal rates of NovoLog  
48 insulin infusion in the pump. This will give the best glucose control and will help you  
49 avoid hyperglycemia (high blood sugar) and ketoacidosis (too much acid [low pH] in  
50 your body).
- 51
- 52 • Glucose monitoring is recommended for all patients who use insulin.

53

54 If you use NovoLog by injection, you may need to increase some or all of the following:

55

- your total dose of insulin
- your dose of intermediate or long-acting insulin (for example, NPH)
- the number of injections of basal insulin

56

57

58

59 If you infuse NovoLog into the skin (subcutaneous tissue) by pump, you may need to  
60 increase some or all of the following:

61

- your total insulin dose
- the basal infusion dose
- the proportion of total insulin given as a basal infusion

62

63

64

65 Age and exposure to heat affect the stability of NovoLog and its preservative. Also,  
66 NovoLog does not work well after it has been frozen. Therefore, do not use old insulin or  
67 insulin that has been exposed to temperature extremes. Hyperglycemia may be a sign that  
68 the insulin is no longer working and needs to be replaced.

69

70

**Do not mix NovoLog:**

71

- with any other insulins when used in a pump
- with Lantus<sup>®</sup> (insulin glargine [rDNA origin] injection) when used with injections  
by syringe

72

(You may, however, mix NovoLog with NPH when used with injections by syringe.  
See: How should I mix insulins?)

73

74

75

76

***For Pump Users***

77

78 • Glucose monitoring is very important for patients using external pump subcutaneous  
79 infusion therapy. You should be aware that pump or infusion set malfunctions that  
80 result in inadequate insulin infusion can quickly lead to hyperglycemia and ketosis.  
81 Accordingly, problems with the infusion pump, the flow of insulin, or the quality of  
82 the insulin should be identified and corrected as quickly as possible. There is only a  
83 small amount of insulin infused into the skin with a pump. The faster absorption  
84 through the skin of rapid-acting insulin analogs and shorter duration of action may  
85 give you less time to identify and correct the problem than with buffered regular  
86 insulin.

87

88

89 • Therefore, you should dose with insulin from a new vial of NovoLog if unexplained  
hyperglycemia or pump alarms do not respond to all of the following:

90

- a repeat dose (injection or bolus) of NovoLog

- 91 • a change in the infusion set, including the NovoLog in the reservoir
- 92 • a change in the infusion site

93

94 If these measures do not work, you may need to resume skin (subcutaneous)  
95 injections with syringes or insulin pens. Continue to monitor your glucose and  
96 ketones. If problems continue, you must contact your doctor.

97

- 98 • When NovoLog is used in an external subcutaneous insulin infusion pump, you  
99 should use only recommended pumps and infusion sets (insulin reservoirs, tubing,  
100 catheters). The infusion set, reservoir insulin, and infusion site should be changed:  
101 • at intervals of 48 hours or less  
102 • with unexpected hyperglycemia or ketosis  
103 • when alarms sound, as specified by your MiniMed or Disetronic pump manual  
104 • if the insulin or pump has been exposed to temperatures over 98.6°F (37°C), as it  
105 might be in a sauna, with long showers, or on a hot day  
106 • if the insulin or pump could have absorbed radiant heat, for example from  
107 sunlight, that would heat the insulin to over 98.6°F (37°C). Dark colored pump  
108 cases or sport covers can increase this type of heat. The location where the pump  
109 is worn may also affect the temperature

110

111 Patients who develop “pump bumps” (skin reactions at the infusion site) may need to  
112 change infusion sites more often.

113

114 **For your safety, read the section “What are the possible side effects of NovoLog?” to**  
115 **review the symptoms of low blood sugar (hypoglycemia) and high blood sugar**  
116 **(hyperglycemia).**

117

### 118 **What is NovoLog?**

119 NovoLog is a clear, colorless, sterile solution for injection or infusion under the skin  
120 (subcutaneously). NovoLog is a human-made form of insulin to lower your blood sugar  
121 faster than human regular insulin. Because the insulin is human-made by recombinant  
122 DNA technology (rDNA) and is chemically different from the insulin made by the human  
123 body, it is called an insulin analog. The active ingredient in NovoLog is insulin aspart.  
124 The concentration of insulin aspart is 100 units per milliliter, or U100. NovoLog also  
125 contains: glycerin, phenol, metacresol, zinc, disodium hydrogen phosphate dihydrate,  
126 and sodium chloride. Hydrochloric acid and/or sodium hydroxide may be added to adjust  
127 the pH. These ingredients help to preserve or stabilize NovoLog insulin. The pH  
128 (balance between acid and alkaline conditions) is important to the stability of NovoLog.  
129 Increases in temperature can affect the stability of NovoLog, so it may not work well.

130

### 131 **Who should not use NovoLog?**

132 Do not use NovoLog if:

- 133 • your blood sugar (glucose) is too low (hypoglycemia)
- 134 • you do not plan to eat right after your injection or infusion

- 135 • you are allergic to insulin aspart or any of the ingredients contained in NovoLog  
136 (check with your doctor if you are not sure)

137

138 The effects of NovoLog on an unborn child or on a nursing baby are unknown.  
139 Therefore, tell your doctor if you plan to become pregnant or breast feed, or if you  
140 become pregnant. You may need to use another medicine.

141

142 Tell your doctor about all medicines and supplements that you are using. Some  
143 medicines, including non-prescription medicines and dietary supplements, may affect  
144 your diabetes.

145

146 **What should I know about using insulin?**

- 147 • Make any change of insulin cautiously and only under medical supervision. Changes  
148 in the strength, manufacturer, type (for example: Regular, NPH, Lente<sup>®</sup>), species  
149 (beef, pork, beef-pork, human) or method of manufacture (recombinant [rDNA] or  
150 animal source insulin) may cause a need for a change in the timing or dose of the new  
151 insulin.
- 152 • Glucose monitoring will help you and your health care provider adjust dosages.
- 153 • Always carry a quick source of sugar, such as candy or glucose tablets, to treat low  
154 blood sugars (hypoglycemia).
- 155 • Always carry identification that states that you have diabetes.

156

157 **What should I know about using NovoLog?**

158 *See the end of this Patient Information for instructions for using NovoLog in*  
159 *injections and pumps.*

160

- 161 • NovoLog starts working 10-20 minutes after injection or infusion. The greatest blood  
162 sugar lowering effect is between 1 and 3 hours after injection or infusion. This blood  
163 sugar lowering lasts for 3 to 5 hours. (The time periods are only general guidelines.)  
164
- 165 • Because the onset of action is rapid, you should eat a meal within 5-10 minutes after a  
166 NovoLog injection or a NovoLog bolus dose from an external pump to avoid low  
167 blood sugar (hypoglycemia).  
168
- 169 • The shorter duration of NovoLog's action means that you may need to use an  
170 intermediate or longer-acting insulin (basal insulin) or higher basal rates of NovoLog  
171 insulin infusion in the pump. This will help you avoid hyperglycemia and  
172 ketoacidosis.  
173
- 174 • Do not inject or infuse in skin that has become reddened or bumpy or thickened after  
175 infusion or injection. Insulin absorption in these areas may not be the same as that in  
176 normal skin, and may change the onset and duration of insulin action.  
177
- 178 • Use NovoLog only if it appears clear and colorless. Do not use NovoLog if it appears  
179 cloudy, thickened, or colored, or if it contains solid particles.

180

181 **What should I avoid while using NovoLog?**

- 182 • Drinking alcohol may lead to hypoglycemia.  
183 • Do not miss meals after injections of NovoLog or bolus infusions of NovoLog.  
184

185 **What are the possible side effects of NovoLog?**

186 Insulins can cause hypoglycemia (low blood sugar), hyperglycemia (high blood sugar),  
187 allergy, and skin reactions.  
188

189 **Hypoglycemia** (insulin reaction). This is the most common side effect. It occurs when  
190 there is a conflict between the amount of carbohydrates (source of glucose) from your  
191 food, the amount of glucose used by your body, and the amount and timing of insulin  
192 dosing. Therefore, **hypoglycemia can occur with:**

- 193 • **The wrong insulin dose.** This can happen with any of the following:  
194 • too much insulin is injected  
195 • the bolus dose of insulin infusion is set too high  
196 • the basal infusion dose is set too high  
197 • the pump does not work right, delivering too much insulin  
198 • **Medicines that directly lower glucose or increase sensitivity to insulin.** This can  
199 happen with oral (taken by mouth) antidiabetes drugs, sulfa antibiotics (for  
200 infections), ACE inhibitors (for blood pressure and heart failure), salicylates,  
201 including aspirin and NSAIDS (for pain), some antidepressants, and with other  
202 medicines.  
203 • **Medical conditions that limit the body's glucose reserve, lengthen the time**  
204 **insulin stays in the body, or that increase sensitivity to insulin.** These conditions  
205 include diseases of the adrenal glands, the pituitary, the thyroid gland, the liver, and  
206 the kidney.  
207 • **Not enough carbohydrate (sugar or starch) intake.** This can happen if:  
208 • a meal or snack is missed or delayed  
209 • you have vomiting or diarrhea that decreases the amount of glucose absorbed by  
210 your body  
211 • alcohol interferes with carbohydrate metabolism  
212 • **Too much glucose use by the body.** This can happen from:  
213 • too much exercise  
214 • higher than normal metabolism rates due to fever or an overactive thyroid  
215

216 Hypoglycemia can be mild or severe. Its onset may be rapid. Patients with very good  
217 (tight) glucose control, patients with diabetic neuropathy (nerve problems), or patients  
218 using some Beta-blockers (used for high blood pressure and heart conditions) may have  
219 few warning symptoms before severe hypoglycemia develops. Hypoglycemia may reduce  
220 your ability to drive a car or use mechanical equipment without risk of injury to yourself  
221 or others. Severe hypoglycemia can cause temporary or permanent harm to your heart or  
222 brain. **It may cause unconsciousness, seizures, or death.** Symptoms of hypoglycemia  
223 include:

- 224 • anxiety, irritability, restlessness, trouble concentrating, personality changes, mood
- 225 changes, or other abnormal behavior
- 226 • tingling in your hands, feet, lips, or tongue
- 227 • dizziness, light-headedness, or drowsiness
- 228 • nightmares or trouble sleeping
- 229 • headache
- 230 • blurred vision or slurred speech
- 231 • palpitations (rapid heart beat)
- 232 • sweating
- 233 • tremor (shaking) or unsteady gait (walking)

234

235 Mild to moderate hypoglycemia can be treated by eating or drinking carbohydrates (milk,  
236 orange juice, sugar candies, or glucose tablets). More severe or continuing hypoglycemia  
237 may require the help of another person or emergency medical personnel. Patients who are  
238 unable to take sugar by mouth or who are unconscious may need treatment with a  
239 glucagon injection or glucose given intravenously (in the vein).

240

241 Talk with your doctor about severe, continuing, or frequent hypoglycemia, and  
242 hypoglycemia for which you had few warning symptoms.

243

244 **Hyperglycemia** (high blood sugar) is another common side effect. It also occurs when  
245 there is a conflict between the amount of carbohydrates (source of glucose) from your  
246 food, the amount of glucose used by your body, and the amount and timing of insulin  
247 dosing. Therefore, **hyperglycemia can occur with:**

- 248 • **The wrong insulin dose.** This can happen from any of the following:
  - 249 • too little or no insulin is injected
  - 250 • the bolus dose of insulin infusion is set too low
  - 251 • the basal infusion dose is set too low
  - 252 • the pump or catheter system does not work right, delivering too little insulin
  - 253 • the insulin's ability to lower glucose is changed by incorrect storage (freezing,  
254 excessive heat), or usage after the expiration date
- 255 • **Medicines that directly increase glucose or decrease sensitivity to insulin.** This  
256 can happen, for example, with thiazide water pills (used for blood pressure),  
257 corticosteroids, birth control pills, and protease inhibitors (used for AIDS).
- 258 • **Medical conditions that increase the body's production of glucose or decrease**  
259 **sensitivity to insulin.** These medical conditions include fevers, infections, heart  
260 attacks, and stress.
- 261 • **Too much carbohydrate intake.** This can happen if you
  - 262 • eat larger meals
  - 263 • eat more often
  - 264 • increase the proportion of carbohydrate in your meals

265

266 Hyperglycemia can be mild or severe. It can **progress to diabetic acidosis (DKA)**  
267 **(ketoacidosis) or very high glucose levels (hyperosmolar coma) and result in**



268 **unconsciousness and death.** Although diabetic acidosis occurs most often in patients  
269 with Type 1 diabetes, it can occur in patients with Type 2 diabetes who become severely  
270 ill. Urine or blood tests will show acetone, ketones, and high levels of glucose.

271 Hyperosmolar coma occurs most often in patients with Type 2 diabetes. Urine and blood  
272 tests will show very high levels of glucose.

273 Glucose monitoring is very important for patients using external pump infusion therapy.

274 You should be aware that pump or infusion set malfunctions that result in inadequate  
275 insulin infusion can quickly lead to hyperglycemia and ketosis. Accordingly, problems  
276 with the infusion pump, the flow of insulin, or the quality of the insulin should be  
277 identified and corrected as quickly as possible. The faster absorption of rapid-acting  
278 insulin analogs through the skin and shorter duration of action may give you less time to  
279 identify and correct the problem.

280 Because some patients experience few symptoms of hyperglycemia and ketosis, it is  
281 important to monitor your glucose several times a day. Symptoms of hyperglycemia  
282 include:

- 283 • confusion or drowsiness
- 284 • fruity smelling breath
- 285 • rapid, deep breathing
- 286 • increased thirst
- 287 • decreased appetite, nausea, or vomiting
- 288 • abdominal (stomach area) pain
- 289 • rapid heart rate
- 290 • increased urination and dehydration (too little fluid in your body)

291

292 Mild hyperglycemia can be treated by extra doses of insulin and drinking fluids  
293 (rehydration). Patients using pumps should check pump function and replace the insulin  
294 in the reservoir-syringe, as well as change the tubing and catheter and the infusion site.

295 **Patients using pumps may need to resume insulin injections with syringes or**  
296 **injection pens.** Glucose and acetone-ketone levels should be monitored more often until  
297 they return to normal. **More severe or continuing hyperglycemia requires prompt**  
298 **evaluation and treatment by your health care provider.**

299

300 **Allergy can be serious.** Generalized allergy is an uncommon, but possibly life-  
301 threatening, reaction to insulin products. Symptoms include:

- 302 • itchy rash over the entire body
- 303 • shortness of breath or wheezing
- 304 • confusion
- 305 • low blood pressure
- 306 • rapid heart beat
- 307 • sweating

308 **If you think you are having a generalized allergic reaction, get emergency medical**  
309 **help right away.**

310

311 Allergic reactions at the injection site (itching, redness, hardness, or swelling) are more  
312 common than generalized allergy. They may need several days or weeks to clear up.

313 Pump patients with site reactions may need to change their infusion sites more often than  
314 every 48 hours. Patients should avoid injection or infusion of insulin into skin areas that  
315 have reactions. Tell your doctor about such reactions, because they can become more  
316 severe, or they may change the absorption of insulin.

317

318 **Lipodystrophy** is a common change in the fat below the injection site. These changes  
319 include loss of fat (depressions in the skin called lipoatrophy) or thickening of the tissue  
320 under the skin (lipohypertrophy). Pump patients with lipodystrophy may need to change  
321 their infusion sites more often than every 48 hours. Patients should avoid injection or  
322 infusion of insulin into skin areas that have these reactions. Tell your doctor about such  
323 reactions because they can become more severe, or they may change the absorption of  
324 insulin.

325

### 326 **How should I store NovoLog?**

- 327 • **NovoLog can be damaged by high temperatures.** Therefore, be sure to protect it  
328 from high air temperatures, heat from the sun, saunas, long showers, and other heat  
329 sources. This is especially important if you use a pump or an insulin pen, because  
330 you carry these devices with you and they may be exposed to different temperatures  
331 as you go about your daily activities. **Throw NovoLog away if it has been in**  
332 **temperatures greater than 98.6°F (37°C).**
- 333
- 334 • **Unopened NovoLog** should be stored in a refrigerator but not in the freezer and  
335 protected from light. Even if it has been refrigerated and protected from sunlight and  
336 unopened, it should not be used after the expiration date on the label and the carton.  
337 Unopened vials and cartridges can be stored unrefrigerated at temperatures below  
338 86°F (30°C) and protected from light for up to 28 days.
- 339
- 340 • **Punctured vials and cartridges** can be stored unrefrigerated at temperatures below  
341 86°F (30°C) and protected from light for up to 28 days. Punctured vials may be  
342 stored in the refrigerator. Cartridges inserted into their NovoPen<sup>®</sup> 3 device should not  
343 be stored in the refrigerator.
- 344
- 345 • **The NovoLog in the pump reservoir and the complete infusion set** (reservoir,  
346 tubing, catheter-needle) should be replaced **at least every 48 hours.** Replacement  
347 should be more often than every 48 hours if you have hyperglycemia, the pump alarm  
348 sounds, or the insulin flow is blocked (occlusion).
- 349
- 350 • Never use NovoLog if it has been stored improperly.

351

### 352 **General advice**

353 This leaflet summarizes the most important information about NovoLog. If you would  
354 like more information, talk with your doctor. You can ask your pharmacist or doctor for  
355 information about NovoLog that is written for health professionals.

356

357 **Injection and pump infusion instructions**

- 358 • NovoLog comes in 10 mL (milliliter) vials or in 3 mL cartridges. NovoLog can be  
359 withdrawn from vials with syringes for injection or for insertion into the reservoirs of  
360 external subcutaneous infusion pumps (Disetronic H-TRON<sup>®</sup> plus V100 or MiniMed  
361 Models 505, 506, or 507).
- 362 • Doses of insulin are measured in units. NovoLog is available as a U-100 insulin.  
363 One milliliter (mL) of U-100 contains 100 units of insulin aspart (1 mL=1 cc). Only  
364 U-100 type syringes should be used for injection to ensure proper dosing.
- 365 • Disposable syringes and needles are sterile if the package is sealed. They should be  
366 used only once and thrown away properly, to protect others from harm.
- 367 • NovoLog PenFill<sup>®</sup> 3 mL cartridges are for use with the NovoPen 3, NovoPen 3 Demi,  
368 and NovoPen Junior Insulin Delivery Devices and NovoFine<sup>®</sup> disposable needles.  
369 Never share needles.

370

371 **How should I inject NovoLog?**

372

373 *Using Vials*

- 374 1. The vial and the insulin should be inspected. The insulin should be clear and colorless.  
375 The tamper-resistant cap should be in place to be removed by you. If the cap had been  
376 removed before your first use of the vial, or if the insulin is cloudy or colored, you  
377 should return the vial to the pharmacy. Do not use it.
- 378 2. Both the injection site and your hands should be cleaned with soap and water or with  
379 alcohol. The injection site should be dry before you inject.
- 380 3. The rubber stopper should be wiped with an alcohol wipe.
- 381 4. The plunger of the syringe should be pulled back until the black tip is at the level for  
382 the number of units to be injected.
- 383 5. Insert the needle of the syringe through the rubber stopper of the vial. Push in the  
384 syringe plunger completely to put air into the vial.
- 385 6. Turn the vial upside-down with the needle-syringe still attached, and pull the plunger  
386 back a few units past the correct dose.
- 387 7. Remove any air bubbles by flicking the syringe and squirting air bubbles out the  
388 needle. Continue pushing the plunger until you have the correct dose.
- 389 8. Lift the vial off the syringe.
- 390 9. Inject NovoLog into the subcutaneous (under the skin) tissue (not into muscle or  
391 blood vessels) in the abdomen, thighs, upper arms, or buttocks. Pinch the skin fold  
392 between your fingers and push the needle straight into the pinched skin. Because  
393 insulin absorption and activity can be affected by the site you choose, you should  
394 discuss the injection site with your doctor.
- 395 10. Release the pinched skin and push the plunger in completely. Keep the needle in the  
396 skin for a few seconds before withdrawing the syringe.
- 397 11. Press the injection site for a few seconds to reduce bleeding. Do not rub.
- 398 12. To avoid needle sticks, throw away the syringe and needle without recapping. Discuss  
399 sterile technique and proper disposal of your used insulin supplies with your doctor.

400

401 *Using Cartridges*

- 402 1. The cartridge and the insulin should be inspected. The insulin should be clear and  
403 colorless. The tamper-resistant foil should be in place to be removed by you. If the  
404 foil had been punctured or removed before your first use of the cartridge or if the  
405 insulin is cloudy or colored, you should return the cartridge to the pharmacy. Do not  
406 use it.
- 407 2. Both the injection site and your hands should be cleaned with soap and water or with  
408 alcohol. The injection site should be dry before you inject. Do not use skin that is  
409 reddened, itchy, or thickened as an infusion site.
- 410 3. Insert a 3 mL cartridge in the pen-device barrel. Attach a new needle to the end of the  
411 cartridge and turn the pen device upside-down so that any air bubbles can be  
412 eliminated by flicking the pen device and squirting air bubbles out the needle. (This  
413 should eliminate extra air for all future doses from that cartridge. However, the needle  
414 will need to be changed for each dose.)
- 415 4. Set the dose to be delivered by twisting the top of the pen-device until the correct  
416 number appears in the window.
- 417 5. Inject NovoLog into the subcutaneous (under the skin) tissue (not into muscle or  
418 blood vessels) in the abdomen, thighs, upper arms, or buttocks. Pinch the skin fold  
419 between your fingers and push the needle straight into the pinched skin. Because  
420 insulin absorption and activity can be affected by the site you choose, you should  
421 discuss the injection site with your doctor.
- 422 6. Release the pinched skin. Inject the dose by pressing the flat plunger button on the  
423 top of the pen-device. Keep the needle in the skin for a few seconds before  
424 withdrawing the pen-device.
- 425 7. Press the injection site for a few seconds to reduce bleeding. Do not rub.
- 426 8. Throw away the disposable needle without recapping to avoid needle sticks. Discuss  
427 sterile technique and proper disposal of your used insulin supplies with your doctor.
- 428

429 **How should I infuse NovoLog with an external subcutaneous insulin infusion pump?**

430

431 NovoLog is recommended for use with the Disetronic H-TRON<sup>®</sup> plus V100 and  
432 MiniMed 505, 506, and 507 pumps. The Disetronic 3.15 plastic cartridge and Tenders or  
433 Classic tubing can be used with the Disetronic pump. The MiniMed 3 mL syringe and  
434 Polyfin<sup>®</sup> or Sof-set<sup>®</sup> tubing can be used in the MiniMed pumps. The use of NovoLog in  
435 quick-release infusion sets and cartridge adapters has not been assessed.

436

- 437 1. Inspect your insulin as you would for an injection. The insulin should be clear and  
438 colorless and without particles. The tamper-resistant cap should be in place to be  
439 removed by you. If the cap had been removed before your first use of the vial or if the  
440 insulin is cloudy or colored, you should return the vial to the pharmacy. Do not use it.
- 441 2. Both the infusion site and your hands should be cleaned with soap and water or with  
442 alcohol. The infusion site should be dry before you insert the catheter-needle and  
443 tubing. Do not use skin that is reddened, itchy, bumpy or thickened as an infusion site  
444 because the onset and duration of NovoLog action may not be the same as that in  
445 normal skin.

- 446 3. Fill the reservoir-syringe with 2 days worth of NovoLog plus about 25 extra units to  
447 prime the pump and fill up the dead space of the infusion tubing.
- 448 4. Remove air bubbles from the reservoir according to the pump manufacturers'  
449 instructions.
- 450 5. Attach the infusion set to the reservoir. Make sure the connection is tight. Prime the  
451 infusion set until you see a drop of insulin coming out of the infusion needle-catheter.  
452 Flick the tubing to remove air bubbles. Follow the pump manufacturers' instructions  
453 for additional priming.
- 454 6. Prime the needle-catheter and insert the infusion set into the skin according to the  
455 pump manufacturer.
- 456 7. Program the pump for mealtime NovoLog boluses and NovoLog basal insulin  
457 infusion according to instructions from your doctor and the manufacturer of your  
458 pump equipment.
- 459 8. Change the infusion site, the insulin reservoir, the tubing, the catheter-needle, and the  
460 insulin every 48 hours or less, even if you have not used all of the insulin. This will  
461 help ensure that NovoLog and the pump works well. (See "What is the most  
462 important information I should know about NovoLog?")
- 463 9. Change the infusion site, the insulin reservoir, the tubing, the catheter-needle, and the  
464 insulin if you experience a pump alarm, catheter blockage, hyperglycemia, or if your  
465 pump insulin has been exposed to heat greater than 98.6°F (37°C). (See "What is the  
466 most important information I should know about NovoLog?") Hyperglycemia  
467 identified with glucose monitoring may be the first indication of a problem with the  
468 pump, infusion set, or NovoLog. Hyperglycemia in the absence of an alarm still  
469 requires you to investigate because pump alarms are designed to detect back-pressure  
470 and occlusion. The alarms may not detect all the changes to NovoLog that could  
471 result in hyperglycemia. You may need to resume subcutaneous insulin injections if  
472 the cause of the problem cannot be promptly identified or fixed. (See  
473 "Hyperglycemia" under "What are the possible side effects of NovoLog?")  
474 Remember that long stretches of tubing increase the risk for kinking and expose the  
475 insulin in the tubing to more variations in temperature.

476  
477 **These instructions give you specific information for use of NovoLog in external**  
478 **subcutaneous infusion pumps, but are not a substitute for pump education.**  
479

480 *How should I mix insulins?*  
481

482 **NovoLog should be mixed only when syringe injections are used.** NovoLog can be  
483 mixed with NPH human insulin immediately before use. The NovoLog should be drawn  
484 into the syringe before the NPH. Mixing with other insulins has not been studied.

485 **NovoLog should not be mixed with Lantus® (insulin glargine [rDNA origin]**  
486 **injection). Mixed insulins should NEVER be used in a pump or for intravenous**  
487 **infusion.**  
488

- 489 1. Add together the doses of NPH and NovoLog. The total dose will determine the final  
490 volume in the syringe after drawing up both insulins into the syringe.
- 491 2. Roll the NPH vial between your hands until the liquid is equally cloudy throughout.

- 492 3. Draw into the syringe the same amount of air as the NPH dose. Inject this air into the  
493 NPH vial and then remove the needle without withdrawing or touching any of the  
494 NPH insulin. (Transferring NPH to the NovoLog vial will contaminate the NovoLog  
495 vial and may change how quickly it works.)
- 496 4. Draw into the syringe the same amount of air as the NovoLog dose. Inject this air into  
497 the NovoLog vial. With the needle in place, turn the vial upside-down and withdraw  
498 the correct dose of NovoLog. The tip of the needle must be in the NovoLog to get the  
499 full dose and not an air dose.
- 500 5. Insert the needle into the NPH vial. Turn the NPH vial upside down with the syringe-  
501 needle still in it. Withdraw the correct dose of NPH.
- 502 6. Inject immediately to reduce changes in how quickly the insulin works.

503

504

505 Helpful information for people with diabetes is published by the American Diabetes  
506 Association, 1660 Duke Street, Alexandria, VA 22314

507

508 For information contact:

509 Novo Nordisk Pharmaceuticals Inc.,

510 100 College Road West

511 Princeton, New Jersey 08540

512 1-800-727-6500

513 [www.novonordisk-us.com](http://www.novonordisk-us.com)

514

515 Manufactured by

516 Novo Nordisk A/S

517 2880 Bagsvaerd, Denmark

518

519 License under U.S. Patent No. 5,618,913 and Des. 347,894

520

521 NovoLog<sup>®</sup>, PenFill<sup>®</sup>, NovoPen<sup>®</sup>, NovoFine<sup>®</sup>, and Lente<sup>®</sup> are trademarks of Novo  
522 Nordisk A/S.

523 Lantus<sup>®</sup> is a trademark of Aventis Pharmaceuticals Inc.

524 Polyfin<sup>®</sup> and Sofset<sup>®</sup> are trademarks of Medtronic MiniMed, Inc.

525 H-TRON<sup>®</sup> is a trademark of Disetronic Medical Systems, Inc.

526

527 Date of Issue: December 21, 2001

528

529 8-XXXX-XX-XXX-X

530

531 Printed in Denmark

532

533

-----  
**This is a representation of an electronic record that was signed electronically and  
this page is the manifestation of the electronic signature.**  
-----

/s/

-----  
David Orloff

4/11/02 07:25:56 PM