

BYETTA[®]

exenatide injection

DESCRIPTION

BYETTA[®] (exenatide) is a synthetic peptide that has incretin-mimetic actions and was originally identified in the lizard *Heloderma suspectum*. BYETTA enhances glucose-dependent insulin secretion by the pancreatic beta-cell, suppresses inappropriately elevated glucagon secretion, and slows gastric emptying. Exenatide differs in chemical structure and pharmacological action from insulin, sulfonylureas (including D-phenylalanine derivatives and meglitinides), biguanides, thiazolidinediones, and alpha-glucosidase inhibitors.

Exenatide is a 39-amino acid peptide amide. Exenatide has the empirical formula $C_{184}H_{282}N_{50}O_{60}S$ and molecular weight of 4186.6 Daltons. The amino acid sequence for exenatide is shown below.

H-His-Gly-Glu-Gly-Thr-Phe-Thr-Ser-Asp-Leu-Ser-Lys-Gln-Met-Glu-Glu-Glu-Ala-Val-Arg-Leu-Phe-Ile-Glu-Trp-Leu-Lys-Asn-Gly-Gly-Pro-Ser-Ser-Gly-Ala-Pro-Pro-Pro-Ser-NH₂

BYETTA is supplied for subcutaneous (SC) injection as a sterile, preserved isotonic solution in a glass cartridge that has been assembled in a pen-injector (pen). Each milliliter (mL) contains 250 micrograms (mcg) synthetic exenatide, 2.2 mg metacresol as an antimicrobial preservative, mannitol as a tonicity-adjusting agent, and glacial acetic acid and sodium acetate trihydrate in water for injection as a buffering solution at pH 4.5. Two prefilled pens are available to deliver unit doses of 5 mcg or 10 mcg. Each prefilled pen will deliver 60 doses to provide 30 days of twice daily administration (BID).

CLINICAL PHARMACOLOGY

Mechanism of Action

Incretins, such as glucagon-like peptide-1 (GLP-1), enhance glucose-dependent insulin secretion and exhibit other antihyperglycemic actions following their release into the circulation from the gut. Exenatide is an incretin mimetic agent that mimics the enhancement of glucose-dependent insulin secretion and several other antihyperglycemic actions of incretins.


The amino acid sequence of exenatide partially overlaps that of human GLP-1. Exenatide has been shown to bind and activate the known human GLP-1 receptor *in vitro*. This leads to an increase in both glucose-dependent synthesis of insulin, and *in vivo* secretion of insulin from pancreatic beta cells, by mechanisms involving cyclic AMP and/or other intracellular signaling pathways. Exenatide promotes insulin release from beta cells in the presence of elevated glucose concentrations. When administered *in vivo*, exenatide mimics certain antihyperglycemic actions of GLP-1.

BYETTA improves glycemic control by reducing fasting and postprandial glucose concentrations in patients with type 2 diabetes through the actions described below.

Glucose-dependent insulin secretion: BYETTA has acute effects on pancreatic beta-cell responsiveness to glucose and leads to insulin release only in the presence of elevated glucose concentrations. This insulin secretion subsides as blood glucose concentrations decrease and approach euglycemia.

First-phase insulin response: In healthy individuals, robust insulin secretion occurs during the first 10 minutes following intravenous (IV) glucose administration. This secretion, known as the “first-phase insulin response,” is characteristically absent in patients with type 2 diabetes. The loss of the first-phase insulin response is an early beta-cell defect in type 2 diabetes. Administration of BYETTA at therapeutic plasma concentrations restored first-phase insulin response to an IV bolus of glucose in patients with type 2 diabetes (Figure 1). Both first-phase insulin secretion and second-phase insulin secretion were significantly increased in patients with type 2 diabetes treated with BYETTA compared with saline ($p < 0.001$ for both).

Figure 1: Mean (+SEM) Insulin Secretion Rate During Infusion of BYETTA or Saline in Patients With Type 2 Diabetes and During Infusion of Saline in Healthy Subjects

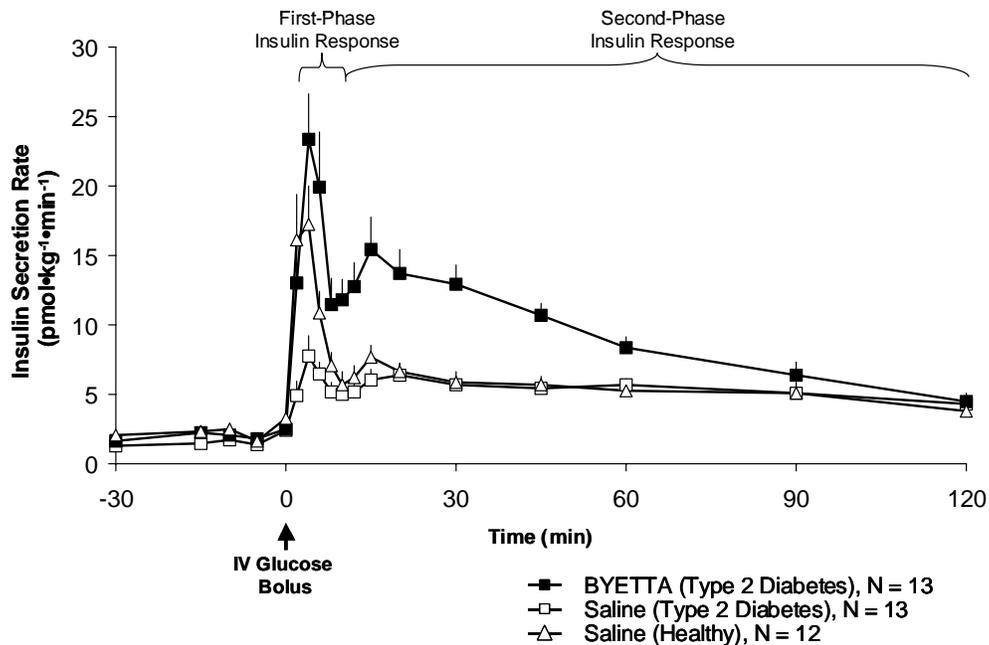

Patients received an IV infusion of insulin for 6.5 h (discontinued at time [t] = -30 min) to normalize plasma glucose concentrations and a continuous IV infusion of either BYETTA or saline for 5 h beginning 3 h prior to an IV bolus of glucose (0.3 g/kg over 30 sec) at t = 0 min.

Glucagon secretion: In patients with type 2 diabetes, BYETTA moderates glucagon secretion and lowers serum glucagon concentrations during periods of hyperglycemia. Lower glucagon concentrations lead to decreased hepatic glucose output and decreased insulin demand. However, BYETTA does not impair the normal glucagon response to hypoglycemia.

Gastric emptying: BYETTA slows gastric emptying, thereby reducing the rate at which meal-derived glucose appears in the circulation.

Food intake: In both animals and humans, administration of exenatide has been shown to reduce food intake.

Pharmacokinetics

Absorption

Following SC administration to patients with type 2 diabetes, exenatide reaches median peak plasma concentrations in 2.1 h. Mean peak exenatide concentration (C_{max}) was 211 pg/mL and overall mean area under the curve (AUC_{0-inf}) was 1036 pg•h/mL following SC administration of a 10 mcg dose of BYETTA. Exenatide exposure (AUC) increased proportionally over the therapeutic dose range of 5 mcg to 10 mcg. The C_{max} values increased less than proportionally over the same range. Similar exposure is achieved with SC administration of BYETTA in the abdomen, thigh, or arm.

Distribution

The mean apparent volume of distribution of exenatide following SC administration of a single dose of BYETTA is 28.3 L.

Metabolism and Elimination

Nonclinical studies have shown that exenatide is predominantly eliminated by glomerular filtration with subsequent proteolytic degradation. The mean apparent clearance of exenatide in humans is 9.1 L/h and the mean terminal half-life is 2.4 h. These pharmacokinetic characteristics of exenatide are independent of the dose. In most individuals, exenatide concentrations are measurable for approximately 10 h post-dose.

Special Populations

Renal Insufficiency

In patients with mild to moderate renal impairment (creatinine clearance 30 to 80 mL/min), exenatide clearance was only mildly reduced; therefore, no dosage adjustment of BYETTA is required in patients with mild to moderate renal impairment. However, in patients with end-stage renal disease receiving dialysis, mean exenatide clearance is reduced to 0.9 L/h compared with 9.1 L/h in healthy subjects (see PRECAUTIONS, General).

Hepatic Insufficiency

No pharmacokinetic study has been performed in patients with a diagnosis of acute or chronic hepatic insufficiency. Because exenatide is cleared primarily by the kidney, hepatic dysfunction is not expected to affect blood concentrations of exenatide (see Pharmacokinetics, Metabolism and Elimination).

Geriatric

Population pharmacokinetic analysis of patients (range from 22 to 73 years) suggests that age does not influence the pharmacokinetic properties of exenatide.

Pediatric

Exenatide has not been studied in pediatric patients.

Gender

Population pharmacokinetic analysis of male and female patients suggests that gender does not influence the distribution and elimination of exenatide.

Race

Population pharmacokinetic analysis of patients including Caucasian, Hispanic, and Black, suggests that race has no significant influence on the pharmacokinetics of exenatide.

Obesity

Population pharmacokinetic analysis of obese ($\text{BMI} \geq 30 \text{ kg/m}^2$) and non-obese patients suggests that obesity has no significant effect on the pharmacokinetics of exenatide.

Drug Interactions

Digoxin

Coadministration of repeated doses of BYETTA (10 mcg BID) decreased the C_{max} of oral digoxin (0.25 mg QD) by 17% and delayed the T_{max} by approximately 2.5 h; however, the overall steady-state pharmacokinetic exposure (AUC) was not changed.

Lovastatin

Lovastatin AUC and C_{max} were decreased approximately 40% and 28%, respectively, and T_{max} was delayed about 4 h when BYETTA (10 mcg BID) was administered concomitantly with a single dose of lovastatin (40 mg) compared with lovastatin administered alone. In the 30-week controlled clinical trials of BYETTA, the use of BYETTA in patients already receiving HMG CoA reductase inhibitors was not associated with consistent changes in lipid profiles compared to baseline.

Lisinopril

In patients with mild to moderate hypertension stabilized on lisinopril (5 to 20 mg/day), BYETTA (10 mcg BID) did not alter steady-state C_{max} or AUC of lisinopril. Lisinopril steady-state T_{max} was delayed by 2 h. There were no changes in 24-h mean systolic and diastolic blood pressure.

Acetaminophen

When 1000 mg acetaminophen elixir was given with 10 mcg BYETTA (0 h) and 1 h, 2 h, and 4 h after BYETTA injection, acetaminophen AUCs were decreased by 21%, 23%, 24%, and 14%, respectively; C_{max} was decreased by 37%, 56%, 54%, and 41%, respectively; T_{max} was increased from 0.6 h in the control period to 0.9 h, 4.2 h, 3.3 h, and 1.6 h, respectively. Acetaminophen AUC, C_{max} and T_{max} were not significantly changed when acetaminophen was given 1 h before BYETTA injection.

Warfarin


Coadministration of repeat doses of BYETTA (5 mcg BID on days 1-2 and 10 mcg BID on days 3-9) in healthy volunteers, delayed warfarin (25 mg) T_{max} by about 2 h. No clinically relevant effects on C_{max} or AUC of S- and R-enantiomers of warfarin were observed. BYETTA did not change the pharmacodynamic properties (as assessed by INR response) of warfarin.

Pharmacodynamics

Postprandial Glucose

In patients with type 2 diabetes, BYETTA reduces the postprandial plasma glucose concentrations (Figure 2).

Figure 2: Mean (+SEM) Postprandial Plasma Glucose Concentrations on Day 1 of BYETTA^a Treatment in Patients With Type 2 Diabetes Treated With Metformin, a Sulfonylurea, or Both (N = 54)

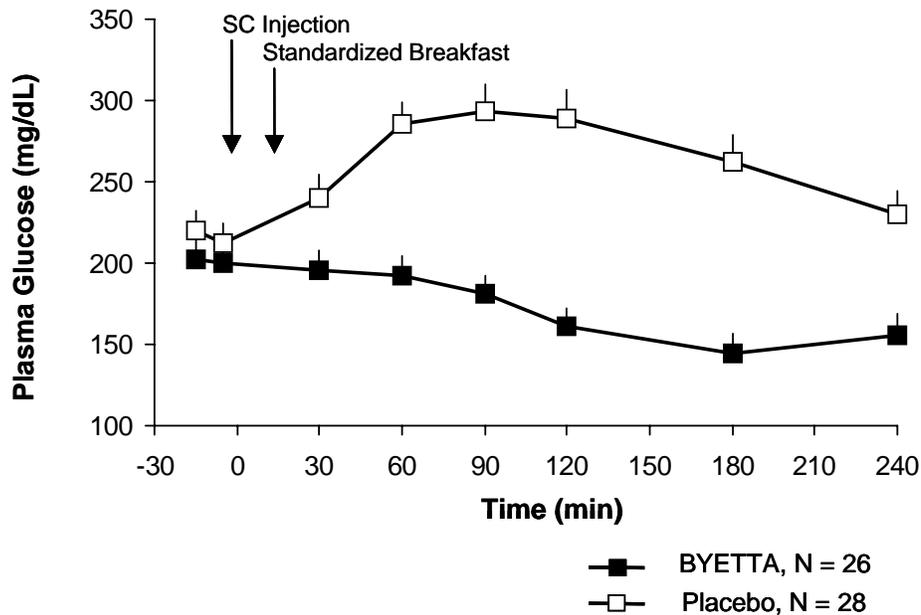


^a Mean dose (7.8 mcg based on body weight) was administered by subcutaneous (SC) injection.

Fasting Glucose

In a single-dose crossover study in patients with type 2 diabetes and fasting hyperglycemia, an immediate insulin release followed injection of BYETTA. Plasma glucose concentrations were significantly reduced with BYETTA compared with placebo (Figure 3).

Figure 3: Mean (+SEM) Serum Insulin and Plasma Glucose Concentrations Following a One-Time Injection of BYETTA^a or Placebo in Fasting Patients With Type 2 Diabetes (N = 12)

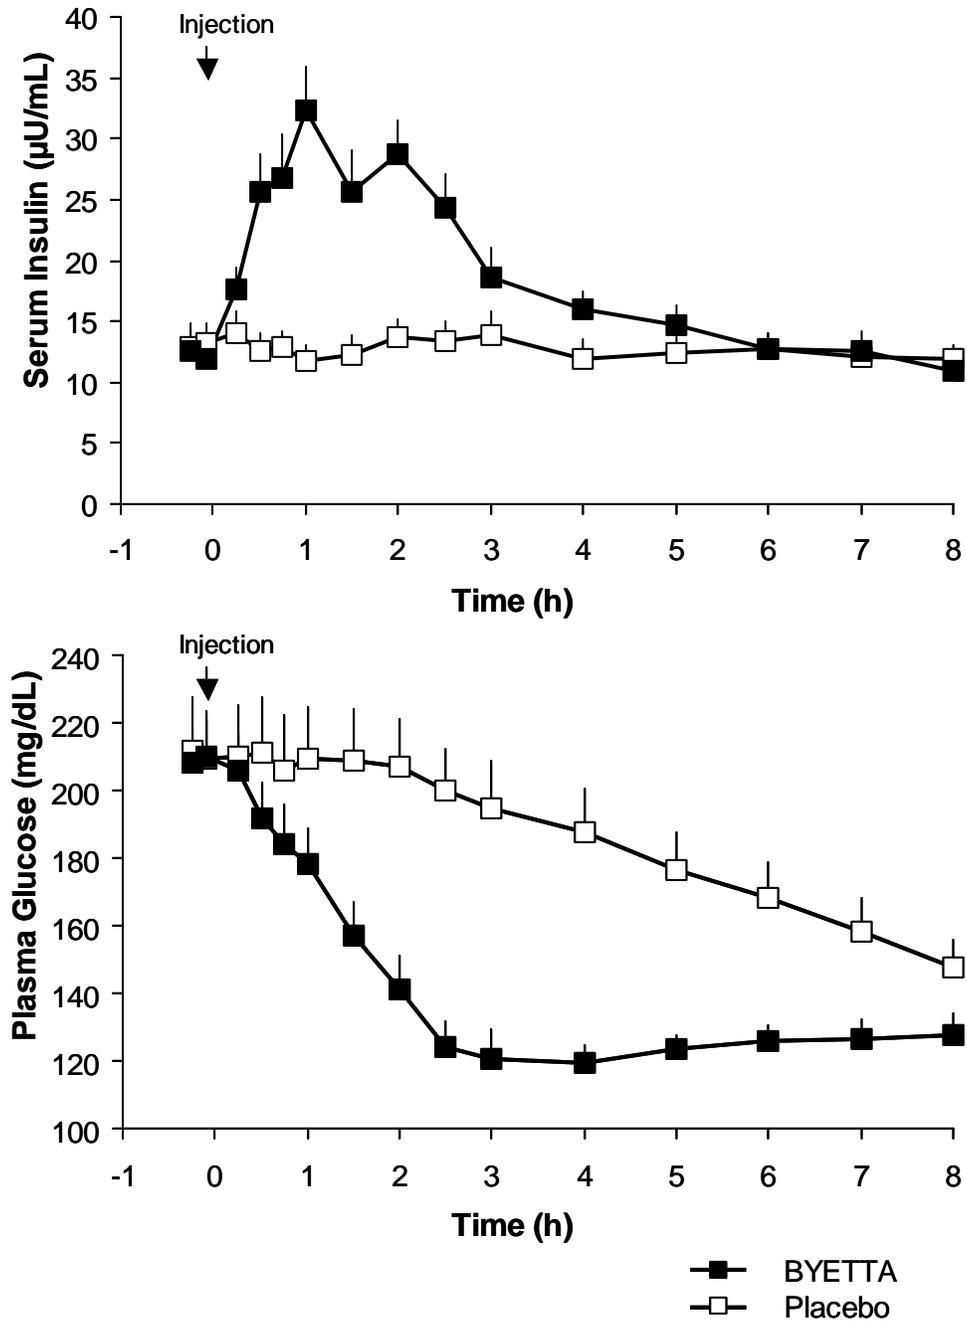

^a BYETTA administration was based on body weight at baseline; mean dose was 9.1 mcg.

CLINICAL STUDIES

Use with metformin and/or a sulfonylurea

Three 30-week, double-blind, placebo-controlled trials were conducted to evaluate the safety and efficacy of BYETTA in patients with type 2 diabetes whose glycemic control was inadequate with metformin alone, a sulfonylurea alone, or metformin in combination with a sulfonylurea.

A total of 1446 patients were randomized in these three trials: 991 (68.5%) were Caucasian, 224 (15.5%) were Hispanic, and 174 (12.0%) were Black. Mean HbA_{1c} values at baseline for the trials ranged from 8.2% to 8.7%. After a 4-week placebo lead-in period, patients were randomly assigned to receive BYETTA 5 mcg BID, BYETTA 10 mcg BID, or placebo BID before the morning and evening meals, in addition to their existing oral antidiabetic agent. All patients assigned to BYETTA began a treatment initiation period with 5 mcg BID for 4 weeks. After 4 weeks, those patients either continued to receive BYETTA 5 mcg BID or had their dose increased to 10 mcg BID. Patients assigned to placebo received placebo BID throughout the study.

The primary endpoint in each study was mean change from baseline HbA_{1c} at 30 weeks. Thirty-week study results are summarized in Table 1.

Table 1: Results of Thirty-Week Placebo-Controlled Trials of BYETTA in Patients With Inadequate Glucose Control Despite the Use of Metformin, a Sulfonylurea, or Both

	Placebo BID	BYETTA 5 mcg BID	BYETTA 10 mcg* BID
	In Combination With Metformin		
Intent-to-Treat Population (N)	113	110	113
HbA_{1c} (%), Mean			
Baseline	8.2	8.3	8.2
Change at Week 30	+0.1	-0.4 [†]	-0.8 [‡]
Proportion Achieving HbA_{1c} ≤7%[§]	13.0%	31.6% [†]	46.4% [†]
Body Weight (kg), Mean			
Baseline	99.9	100.0	100.9
Change at Week 30	-0.3	-1.6 [†]	-2.8 [‡]
	In Combination With a Sulfonylurea		
Intent-to-Treat Population (N)	123	125	129
HbA_{1c} (%), Mean			
Baseline	8.7	8.5	8.6
Change at Week 30	+0.1	-0.5 [†]	-0.9 [‡]
Proportion Achieving HbA_{1c} ≤7%[§]	8.8%	32.6% [†]	41.3% [‡]
Body Weight (kg), Mean			
Baseline	99.1	94.9	95.2
Change at Week 30	-0.6	-0.9	-1.6 [†]
	In Combination With Metformin and a Sulfonylurea		
Intent-to-Treat Population (N)	247	245	241
HbA_{1c} (%), Mean			
Baseline	8.5	8.5	8.5
Change at Week 30	+0.2	-0.6 [‡]	-0.8 [‡]
Proportion Achieving HbA_{1c} ≤7%[§]	9.2%	27.4% [‡]	33.5% [‡]
Body Weight (kg), Mean			
Baseline	99.1	96.9	98.4
Change at Week 30	-0.9	-1.6 [†]	-1.6 [†]

* BYETTA 5 mcg twice daily (BID) for 1 month followed by 10 mcg BID for 6 months before the morning and evening meals.

[†] p ≤0.05, treatment vs. placebo

[‡] p ≤0.0001, treatment vs. placebo

[§] Patients eligible for the analysis with baseline HbA_{1c} >7%.

HbA_{1c}

The addition of BYETTA to a regimen of metformin, a sulfonylurea, or both, resulted in statistically significant reductions from baseline HbA_{1c} at Week 30 compared with patients receiving placebo added to these agents in the three controlled trials (Table 1). In addition, a statistically significant dose-effect was observed between 5-mcg and 10-mcg BYETTA groups for the change from baseline HbA_{1c} at Week 30 in the three studies.

Fasting and Postprandial Glucose

Long-term use of BYETTA in combination with metformin, a sulfonylurea, or both, reduced both fasting and postprandial plasma glucose concentrations in a statistically significant, dose-dependent manner through Week 30. A statistically significant reduction from baseline in both mean fasting and postprandial glucose concentrations was observed at Week 30 in both BYETTA groups compared with placebo in data combined from the three controlled trials. The change in fasting glucose concentration at Week 30 compared with baseline was -8 mg/dL for BYETTA 5 mcg BID and -10 mg/dL for BYETTA 10 mcg BID, compared with +12 mg/dL for placebo. The change in 2-h postprandial glucose concentration following administration of BYETTA at Week 30 compared with baseline was -63 mg/dL for 5 mcg BID and -71 mg/dL for 10 mcg BID, compared with +11 mg/dL for placebo.

Proportion of Patients Achieving HbA_{1c} ≤7%

BYETTA in combination with metformin, a sulfonylurea, or both, resulted in a greater, statistically significant proportion of patients achieving an HbA_{1c} ≤7% at Week 30 compared with patients receiving placebo in combination with these agents (Table 1).

Body Weight

In the three controlled trials, a decrease from baseline body weight at Week 30 was associated with BYETTA 10 mcg BID compared with placebo BID in patients with type 2 diabetes (Table 1).

One-Year Clinical Results

The cohort of 163 patients from the 30-week placebo-controlled trials who completed a total of 52 weeks of treatment with BYETTA 10 mcg BID had HbA_{1c} changes from baseline of -1.0% and -1.1% at 30 and 52 weeks of treatment, respectively, with accompanying changes from baseline in fasting plasma glucose of -14.0 mg/dL and -25.3 mg/dL, and body weight changes of -2.6 kg and -3.6 kg. This cohort had baseline values similar to those of the entire controlled-trial population.

Use with a thiazolidinedione

In a randomized, double-blind, placebo-controlled trial of 16 weeks duration, BYETTA (n = 121) or placebo (n = 112) was added to existing thiazolidinedione (pioglitazone or rosiglitazone) treatment, with or without metformin, in patients with type 2 diabetes with inadequate glycemic control. Randomization to BYETTA or placebo was stratified based on whether the patients were receiving metformin. Patients assigned to placebo received placebo BID throughout the study. BYETTA or placebo was injected subcutaneously before the morning and evening meals. Seventy-nine percent of patients were taking a thiazolidinedione and metformin and 21% were taking a thiazolidinedione alone. The majority of patients (84%) were Caucasian, 8% were Hispanic and 3% were Black. The mean baseline HbA_{1c} values were similar for BYETTA and placebo (7.9%). BYETTA treatment was initiated at a dose of 5 mcg BID for 4 weeks then increased to 10 mcg BID for 12 more weeks.

Sixteen-week study results are summarized in Table 2. Compared to placebo, BYETTA resulted in statistically significant reductions in HbA_{1c} from baseline at Week 16. Treatment effects for HbA_{1c} were similar in the two sub-groups defined by underlying treatment stratum (thiazolidinediones alone versus thiazolidinediones plus metformin). The change in fasting serum glucose concentration from baseline to Week 16 was statistically significant compared with placebo (-21 mg/dL for BYETTA 10 mcg BID compared with +4 mg/dL for placebo).

Table 2: Results of 16-Week Placebo-Controlled Trial of BYETTA in Patients With Inadequate Glucose Control Despite the Use of a Thiazolidinedione (TZD) or a Thiazolidinedione plus Metformin

	Placebo BID	BYETTA 10 mcg* BID
	In Combination With a TZD or a TZD plus MET	
Intent-to-Treat Population (N)	112	121
HbA_{1c} (%), Mean		
Baseline	7.9	7.9
Change at Week 16	+0.1	-0.8 [†]
Proportion Achieving HbA_{1c} ≤7%[‡]	16.2%	62.3% [†]
Body Weight (kg), Mean		
Baseline	96.9	97.5
Change at Week 16	-0.2	-1.5 [†]

* BYETTA 5 mcg twice daily (BID) for 1 month followed by 10 mcg BID for 3 months before the morning and evening meals.

[†] p <0.0001, treatment vs. placebo

[‡] Patients eligible for the analysis with baseline HbA_{1c} >7%.

INDICATIONS AND USAGE

BYETTA is indicated as adjunctive therapy to improve glycemic control in patients with type 2 diabetes mellitus who are taking metformin, a sulfonylurea, a thiazolidinedione, a combination of metformin and a sulfonylurea, or a combination of metformin and a thiazolidinedione, but have not achieved adequate glycemic control.

CONTRAINDICATIONS

BYETTA is contraindicated in patients with known hypersensitivity to exenatide or to any of the product components.

PRECAUTIONS

General

BYETTA is not a substitute for insulin in insulin-requiring patients. BYETTA should not be used in patients with type 1 diabetes or for the treatment of diabetic ketoacidosis.

Patients may develop anti-exenatide antibodies following treatment with BYETTA, consistent with the potentially immunogenic properties of protein and peptide pharmaceuticals. Patients receiving BYETTA should be observed for signs and symptoms of hypersensitivity reactions.

In a small proportion of patients, the formation of anti-exenatide antibodies at high titers could result in failure to achieve adequate improvement in glycemic control. If there is worsening glycemic control or failure to achieve targeted glycemic control, alternative antidiabetic therapy should be considered.

The concurrent use of BYETTA with insulin, D-phenylalanine derivatives, meglitinides, or alpha-glucosidase inhibitors has not been studied.

BYETTA is not recommended for use in patients with end-stage renal disease or severe renal impairment (creatinine clearance <30 mL/min; see Pharmacokinetics, Special Populations). In patients with end-stage renal disease receiving dialysis, single doses of BYETTA 5 mcg were not well tolerated due to gastrointestinal side effects.

BYETTA has not been studied in patients with severe gastrointestinal disease, including gastroparesis. Its use is commonly associated with gastrointestinal adverse effects, including nausea, vomiting, and diarrhea. Therefore, the use of BYETTA is not recommended in patients with severe gastrointestinal disease. The development of severe abdominal pain in a patient treated with BYETTA should be investigated because it may be a warning sign of a serious condition.

Hypoglycemia

In the 30-week controlled clinical trials with BYETTA, a hypoglycemia episode was recorded as an adverse event if the patient reported symptoms associated with hypoglycemia with an accompanying blood glucose <60 mg/dL or if symptoms were reported without an accompanying blood glucose measurement. When BYETTA was used in combination with metformin, no increase in the incidence of hypoglycemia was

observed over that of placebo in combination with metformin. In contrast, when BYETTA was used in combination with a sulfonylurea, the incidence of hypoglycemia was increased over that of placebo in combination with a sulfonylurea. Therefore, patients receiving BYETTA in combination with a sulfonylurea may have an increased risk of hypoglycemia. Most episodes of hypoglycemia were mild to moderate in intensity, and all resolved with oral administration of carbohydrate. Hypoglycemia was rarely observed in patients treated with the combination of BYETTA and metformin and was similar in incidence to patients treated with placebo and metformin (Table 3). To reduce the risk of hypoglycemia associated with the use of a sulfonylurea, reduction in the dose of sulfonylurea may be considered (see DOSAGE AND ADMINISTRATION).

Table 3: Incidence (%) of Hypoglycemia* by Concomitant Antidiabetic Therapy

	BYETTA			BYETTA			BYETTA		
	Placebo BID	5 mcg BID	10 mcg BID	Placebo BID	5 mcg BID	10 mcg BID	Placebo BID	5 mcg BID	10 mcg BID
	With Metformin			With a Sulfonylurea			With MET/SFU		
N	113	110	113	123	125	129	247	245	241
Hypoglycemia	5.3%	4.5%	5.3%	3.3%	14.4%	35.7%	12.6%	19.2%	27.8%

* In three 30-week placebo-controlled clinical trials.

BYETTA and placebo were administered before the morning and evening meals.

Abbreviations: BID, twice daily; MET/SFU, metformin and a sulfonylurea.

When used as add-on to a thiazolidinedione, with or without metformin, the incidence of symptomatic mild to moderate hypoglycemia with BYETTA was 11% compared to 7% with placebo.

BYETTA did not alter the counter-regulatory hormone responses to insulin-induced hypoglycemia in a randomized, double-blind, controlled study in healthy subjects.

Information for Patients

Patients should be informed of the potential risks of BYETTA. Patients should also be fully informed about self-management practices, including the importance of proper storage of BYETTA, injection technique, timing of dosage of BYETTA as well as concomitant oral drugs, adherence to meal planning, regular physical activity, periodic blood glucose monitoring and HbA_{1c} testing, recognition and management of hypoglycemia and hyperglycemia, and assessment for diabetes complications.

Patients should be advised to inform their physicians if they are pregnant or intend to become pregnant.

Each dose of BYETTA should be administered as a SC injection in the thigh, abdomen, or upper arm at any time within the 60-minute period **before** the morning and evening meals (or before the two main meals of the day, approximately 6 hours or more apart). BYETTA **should not** be administered after a meal. If a dose is missed, the treatment regimen should be resumed as prescribed with the next scheduled dose.

The risk of hypoglycemia is increased when BYETTA is used in combination with an agent that induces hypoglycemia, such as a sulfonylurea. The symptoms, treatment, and

conditions that predispose development of hypoglycemia should be explained to the patient. While the patient's usual instructions for hypoglycemia management do not need to be changed, these instructions should be reviewed and reinforced when initiating BYETTA therapy, particularly when concomitantly administered with a sulfonylurea (see PRECAUTIONS, Hypoglycemia).

Patients should be advised that treatment with BYETTA may result in a reduction in appetite, food intake, and/or body weight, and that there is no need to modify the dosing regimen due to such effects. Treatment with BYETTA may also result in nausea, particularly upon initiation of therapy (see ADVERSE REACTIONS).

The patient should read the "Information for the Patient" insert and the Pen User Manual before starting BYETTA therapy and review them each time the prescription is refilled. The patient should be instructed on proper use and storage of the pen, emphasizing how and when to set up a new pen and noting that only one setup step is necessary at initial use. The patient should be advised not to share the pen and needles.

Patients should be informed that pen needles are not included with the pen and must be purchased separately. Patients should be advised which needle length and gauge should be used.

Drug Interactions

The effect of BYETTA to slow gastric emptying may reduce the extent and rate of absorption of orally administered drugs. BYETTA should be used with caution in patients receiving oral medications that require rapid gastrointestinal absorption. For oral medications that are dependent on threshold concentrations for efficacy, such as contraceptives and antibiotics, patients should be advised to take those drugs at least 1 h before BYETTA injection. If such drugs are to be administered with food, patients should be advised to take them with a meal or snack when BYETTA is not administered. The effect of BYETTA on the absorption and effectiveness of oral contraceptives has not been characterized.

Warfarin

In a controlled clinical pharmacology study in healthy volunteers, a delay in warfarin T_{max} of about 2 h was observed when warfarin was administered 30 min after BYETTA. No clinically relevant effects on C_{max} or AUC were observed. However, since market introduction there have been some spontaneously reported cases of increased INR (International Normalized Ratio) with concomitant use of warfarin and BYETTA, sometimes associated with bleeding.

Carcinogenesis, Mutagenesis, Impairment of Fertility

A 104-week carcinogenicity study was conducted in male and female rats at doses of 18, 70, or 250 mcg/kg/day administered by bolus SC injection. Benign thyroid C-cell adenomas were observed in female rats at all exenatide doses. The incidences in female rats were 8% and 5% in the two control groups and 14%, 11%, and 23% in the low-, medium-, and high-dose groups with systemic exposures of 5, 22, and 130 times,

respectively, the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on plasma area under the curve (AUC).

In a 104-week carcinogenicity study in mice at doses of 18, 70, or 250 mcg/kg/day administered by bolus SC injection, no evidence of tumors was observed at doses up to 250 mcg/kg/day, a systemic exposure up to 95 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC.

Exenatide was not mutagenic or clastogenic, with or without metabolic activation, in the Ames bacterial mutagenicity assay or chromosomal aberration assay in Chinese hamster ovary cells. Exenatide was negative in the in vivo mouse micronucleus assay.

In mouse fertility studies with SC doses of 6, 68 or 760 mcg/kg/day, males were treated for 4 weeks prior to and throughout mating and females were treated 2 weeks prior to and throughout mating until gestation day 7. No adverse effect on fertility was observed at 760 mcg/kg/day, a systemic exposure 390 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC.

Pregnancy

Pregnancy Category C

Exenatide has been shown to cause reduced fetal and neonatal growth, and skeletal effects in mice at systemic exposures 3 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC. Exenatide has been shown to cause skeletal effects in rabbits at systemic exposures 12 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC. There are no adequate and well-controlled studies in pregnant women. BYETTA should be used during pregnancy only if the potential benefit justifies the potential risk to the fetus.

In female mice given SC doses of 6, 68, or 760 mcg/kg/day beginning 2 weeks prior to and throughout mating until gestation day 7, there were no adverse fetal effects at doses up to 760 mcg/kg/day, systemic exposures up to 390 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC.

In pregnant mice given SC doses of 6, 68, 460, or 760 mcg/kg/day from gestation day 6 through 15 (organogenesis), cleft palate (some with holes) and irregular skeletal ossification of rib and skull bones were observed at 6 mcg/kg/day, a systemic exposure 3 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC.

In pregnant rabbits given SC doses of 0.2, 2, 22, 156, or 260 mcg/kg/day from gestation day 6 through 18 (organogenesis), irregular skeletal ossifications were observed at 2 mcg/kg/day, a systemic exposure 12 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC.

In pregnant mice given SC doses of 6, 68, or 760 mcg/kg/day from gestation day 6 through lactation day 20 (weaning), an increased number of neonatal deaths were observed on postpartum days 2-4 in dams given 6 mcg/kg/day, a systemic exposure

3 times the human exposure resulting from the maximum recommended dose of 20 mcg/day, based on AUC.

Nursing Mothers

It is not known whether exenatide is excreted in human milk. Many drugs are excreted in human milk and because of the potential for clinically significant adverse reactions in nursing infants from exenatide, a decision should be made whether to discontinue producing milk for consumption or discontinue the drug, taking into account the importance of the drug to the lactating woman. Studies in lactating mice have demonstrated that exenatide is present at low concentrations in milk (less than or equal to 2.5% of the concentration in maternal plasma following subcutaneous dosing). Caution should be exercised when BYETTA is administered to a nursing woman.

Pediatric Use

Safety and effectiveness of BYETTA have not been established in pediatric patients.

Geriatric Use

BYETTA was studied in 282 patients 65 years of age or older and in 16 patients 75 years of age or older. No differences in safety or effectiveness were observed between these patients and younger patients.

ADVERSE REACTIONS

Use with metformin and/or a sulfonylurea

In the three 30-week controlled trials of BYETTA add-on to metformin and/or sulfonylurea, adverse events with an incidence $\geq 5\%$ (excluding hypoglycemia; see Table 3) that occurred more frequently in BYETTA-treated patients compared with placebo-treated patients are summarized in Table 4.

Table 4: Frequent Treatment-Emergent Adverse Events ($\geq 5\%$ Incidence and Greater Incidence With BYETTA Treatment) Excluding Hypoglycemia*

	Placebo BID N = 483	All BYETTA BID N = 963
	%	%
Nausea	18	44
Vomiting	4	13
Diarrhea	6	13
Feeling Jittery	4	9
Dizziness	6	9
Headache	6	9
Dyspepsia	3	6

* In three 30-week placebo-controlled clinical trials.

The adverse events associated with BYETTA generally were mild to moderate in intensity. The most frequently reported adverse event, mild to moderate nausea, occurred in a dose-dependent fashion. With continued therapy, the frequency and severity decreased over time in most of the patients who initially experienced nausea. Adverse events reported in ≥ 1.0 to $< 5.0\%$ of patients receiving BYETTA and reported more frequently than with placebo included asthenia (mostly reported as weakness), decreased

appetite, gastroesophageal reflux disease, and hyperhidrosis. Patients in the extension studies at 52 weeks experienced similar types of adverse events observed in the 30-week controlled trials.

The incidence of withdrawal due to adverse events was 7% for BYETTA-treated patients and 3% for placebo-treated patients. The most common adverse events leading to withdrawal for BYETTA-treated patients were nausea (3% of patients) and vomiting (1%). For placebo-treated patients, <1% withdrew due to nausea and 0% due to vomiting.

Use with a thiazolidinedione

In the 16-week placebo-controlled study of BYETTA add-on to a thiazolidinedione, with or without metformin, the incidence and type of other adverse events observed were similar to those seen in the 30-week controlled clinical trials with metformin and/or a sulfonylurea. No serious adverse events were reported in the placebo arm. Two serious adverse events, namely chest pain (leading to withdrawal) and chronic hypersensitivity pneumonitis, were reported in the BYETTA arm.

The incidence of withdrawal due to adverse events was 16% (19/121) for BYETTA-treated patients and 2% (2/112) for placebo-treated patients. The most common adverse events leading to withdrawal for BYETTA-treated patients were nausea (9%) and vomiting (5%). For placebo-treated patients, <1% withdrew due to nausea. Chills (n = 4) and injection-site reactions (n = 2) occurred only in BYETTA-treated patients. The two patients who reported an injection-site reaction had high titers of anti-exenatide antibody.

Spontaneous Data

Since market introduction of BYETTA, the following additional adverse reactions have been reported. Because these events are reported voluntarily from a population of uncertain size, it is not always possible to reliably estimate their frequency or establish a causal relationship to drug exposure.

General: injection-site reactions; dysgeusia; somnolence, INR increased with concomitant warfarin use (some reports associated with bleeding).

Allergy/Hypersensitivity: generalized pruritus and/or urticaria, macular or papular rash, angioedema; rare reports of anaphylactic reaction.

Gastrointestinal: nausea, vomiting, and/or diarrhea resulting in dehydration with some reports associated with increased serum creatinine/acute renal failure that may be reversible if treated appropriately; abdominal distension, abdominal pain, eructation, constipation, flatulence, acute pancreatitis.

Immunogenicity

Consistent with the potentially immunogenic properties of protein and peptide pharmaceuticals, patients may develop anti-exenatide antibodies following treatment with BYETTA. In most patients who develop antibodies, antibody titers diminish over time.

In the 30-week controlled trials of BYETTA add-on to metformin and/or sulfonylurea, 38% of patients had low titer anti-exenatide antibodies at 30 weeks. For this group, the level of glycemic control (HbA_{1c}) was generally comparable to that observed in those without antibody titers. An additional 6% of patients had higher titer antibodies at 30 weeks. In about half of this 6% (3% of the total patients given BYETTA in the 30-week controlled studies), the glycemic response to BYETTA was attenuated; the remainder had a glycemic response comparable to that of patients without antibodies.

In the 16-week trial of BYETTA add-on to thiazolidinediones, with or without metformin, 9% of patients had higher titer antibodies at 16 weeks. Compared with patients who did not develop antibodies to BYETTA, on average the glycemic response in patients with higher titer antibodies was attenuated.

The patient's glycemic response to BYETTA should be monitored. If there is worsening glycemic control or failure to achieve targeted glycemic control, alternative antidiabetic therapy should be considered.

OVERDOSAGE

In a clinical study of BYETTA, three patients with type 2 diabetes each experienced a single overdose of 100 mcg SC (10 times the maximum recommended dose). Effects of the overdoses included severe nausea, severe vomiting, and rapidly declining blood glucose concentrations. One of the three patients experienced severe hypoglycemia requiring parenteral glucose administration. The three patients recovered without complication. In the event of overdose, appropriate supportive treatment should be initiated according to the patient's clinical signs and symptoms.

DOSAGE AND ADMINISTRATION

BYETTA therapy should be initiated at 5 mcg per dose administered twice daily at any time within the 60-minute period before the morning and evening meals (or before the two main meals of the day, approximately 6 hours or more apart). BYETTA should not be administered after a meal. Based on clinical response, the dose of BYETTA can be increased to 10 mcg twice daily after 1 month of therapy. Each dose should be administered as a SC injection in the thigh, abdomen, or upper arm.

BYETTA is recommended for use in patients with type 2 diabetes mellitus who are already receiving metformin, a sulfonylurea, a thiazolidinedione, a combination of metformin and a sulfonylurea, or a combination of metformin and a thiazolidinedione, and have suboptimal glycemic control. When BYETTA is added to metformin or thiazolidinedione therapy, the current dose of metformin or thiazolidinedione can be continued as it is unlikely that the dose of metformin or thiazolidinedione will require adjustment due to hypoglycemia when used with BYETTA. When BYETTA is added to sulfonylurea therapy, a reduction in the dose of sulfonylurea may be considered to reduce the risk of hypoglycemia (see PRECAUTIONS, Hypoglycemia).

BYETTA is a clear and colorless liquid and should not be used if particles appear or if the solution is cloudy or colored. BYETTA should not be used past the expiration date.

No data are available on the safety or efficacy of intravenous or intramuscular injection of BYETTA.

STORAGE

Prior to first use, BYETTA must be stored refrigerated at 36°F to 46°F (2°C to 8°C). After first use, BYETTA can be kept at a temperature not to exceed 77°F (25°C). Do not freeze. Do not use BYETTA if it has been frozen. BYETTA should be protected from light. The pen should be discarded 30 days after first use, even if some drug remains in the pen.

HOW SUPPLIED

BYETTA is supplied as a sterile solution for subcutaneous injection containing 250 mcg/mL exenatide. The following packages are available:

5 mcg per dose, 60 doses, 1.2 mL prefilled pen	NDC 66780-210-07
10 mcg per dose, 60 doses, 2.4 mL prefilled pen	NDC 66780-210-08

Rx ONLY

Manufactured for Amylin Pharmaceuticals, Inc., San Diego, CA 92121
Marketed by Amylin Pharmaceuticals, Inc. and Eli Lilly and Company
1-800-868-1190
<http://www.BYETTA.com>

Literature Revised February 2007

BYETTA is a registered trademark of Amylin Pharmaceuticals, Inc.

© 2007 Amylin Pharmaceuticals, Inc. All rights reserved.

822003-CC

Patient Information

BYETTA[®] (bye-A-tuh) **exenatide injection**

Read this Patient Information and the Pen User Manual that come with BYETTA before you start using it and each time you get a refill. There may be new information. This Patient Information does not take the place of talking with your healthcare provider about your medical condition or your treatment. **If you have questions about BYETTA after reading this information, ask your healthcare provider or pharmacist.**

What is BYETTA?

BYETTA is an injectable medicine used to improve glucose (blood sugar) control in adults with type 2 diabetes. BYETTA can be used with metformin, a sulfonylurea, or a thiazolidinedione. There are many antidiabetic medicines that contain a sulfonylurea. Ask your healthcare provider or pharmacist if you are not sure if your antidiabetic medicine contains a sulfonylurea.

BYETTA is not a substitute for insulin in patients whose diabetes requires insulin treatment. BYETTA has not been studied in children.

Who should not use BYETTA?

Do not use BYETTA if:

- You are allergic to exenatide or any of the other ingredients in BYETTA. See the end of this Patient Information for a complete list of ingredients.

What should I tell my healthcare provider before using BYETTA?

Tell your healthcare provider about all of your medical conditions including if you:

- Have severe problems with your stomach (gastroparesis) or food digestion. BYETTA slows stomach emptying so food passes more slowly through your stomach.
- Have severe kidney disease or you are on dialysis.
- Are pregnant or planning to become pregnant. It is not known if BYETTA may harm your unborn child.

- Are breastfeeding. It is not known if BYETTA passes into your milk and can harm your child.

Tell your healthcare provider about all the medicines you take including prescription and nonprescription medicines, vitamins, and herbal supplements.

BYETTA slows stomach emptying and can affect medicines that need to pass through the stomach quickly. Ask your healthcare provider if the time at which you take any of your oral medicines (for example, birth control pills, antibiotics) should be changed.

Know the medicines you take. Keep a list of them with you to show your healthcare provider and pharmacist each time you get a new medicine.

How should I use BYETTA?

See the accompanying Pen User Manual for instructions for using the BYETTA Pen and injecting BYETTA. BYETTA comes in a prefilled pen. Two prefilled pens (5 mcg or 10 mcg) are available, depending on your prescribed dose (5 mcg or 10 mcg, twice a day). Each pen has 60 doses to provide 30 days of twice-a-day injections. You must do a “New Pen Set-Up” (see User Manual) one time only, when starting a new prefilled BYETTA Pen. If you do this “New Pen Set-Up” before each injection, you will run out of medicine before 30 days.

- Use BYETTA exactly as prescribed by your healthcare provider. Your dose may be increased after using BYETTA for 30 days. Do not change your dose unless your healthcare provider has told you to change your dose. Your healthcare provider must teach you how to inject BYETTA before you use it for the first time. If you have questions or do not understand the instructions, talk to your healthcare provider or pharmacist.
- Pen needles are not included. You may need a prescription to purchase pen needles from your pharmacist. Ask your healthcare provider which needle length and gauge is best for you.
- Inject your dose of BYETTA under the skin (subcutaneous injection) of your upper leg (thigh), stomach area (abdomen), or upper arm.
- BYETTA is injected, twice a day, at any time within the 60 minutes (1 hour) **before** your morning and evening meals (or before the two main meals of the day, approximately 6 hours or more apart). **Do not** take BYETTA after your meal.
- If you miss a dose of BYETTA, skip that dose and take your next dose at the next prescribed time. **Do not** take an extra dose or increase the amount of your next dose to make up for the one you missed.
- If you use too much BYETTA, call your healthcare provider or poison control center right away. You may need medical treatment right away. Too much BYETTA can cause nausea, vomiting, dizziness, or symptoms of low blood sugar.

What are the possible side effects of BYETTA?

When BYETTA is used with a medicine that contains a sulfonylurea, hypoglycemia (low blood sugar) can occur. The dose of your sulfonylurea medicine may need to be reduced while you use BYETTA. The signs and symptoms of low blood sugar may include headache, drowsiness, weakness, dizziness, confusion, irritability, hunger, fast heartbeat, sweating, and feeling jittery. Your healthcare provider should tell you how to treat low blood sugar.

The most common side effects with BYETTA include nausea, vomiting, diarrhea, dizziness, headache, feeling jittery, and acid stomach. Nausea is most common when first starting BYETTA, but decreases over time in most patients.

BYETTA may reduce your appetite, the amount of food you eat, and your weight. No changes in your dose are needed for these side effects.

Talk to your healthcare provider about any side effect that bothers you or that does not go away.

These are not all the side effects with BYETTA. Ask your healthcare provider or pharmacist for more information.

How should I store BYETTA?

- Store your new, unused BYETTA Pen in the original carton in a refrigerator at 36°F to 46°F (2°C to 8°C) protected from light. Do not freeze. Throw away any BYETTA Pen that has been frozen.
- After first use, your BYETTA Pen can be kept at a temperature not to exceed 77°F (25°C). Do not freeze. Do not use BYETTA if it has been frozen. BYETTA should be protected from light.
- Use a BYETTA Pen for only 30 days. Throw away a used BYETTA Pen after 30 days, even if some medicine remains in the pen.
- BYETTA should not be used after the expiration date printed on the label.
- Do not store the BYETTA Pen with the needle attached. If the needle is left on, medicine may leak from the BYETTA Pen or air bubbles may form in the cartridge.
- **Keep your BYETTA Pen, pen needles, and all medicines out of the reach of children.**

General information about BYETTA

Medicines are sometimes prescribed for conditions that are not listed in the Patient Information. Do not use BYETTA for a condition for which it was not prescribed. Do not give BYETTA to other people, even if they have the same symptoms you have. It may harm them.

Your food and exercise plan, along with your periodic blood sugar testing and scheduled A1C (also known as HbA_{1C}) checks, will continue to be important in managing your diabetes while you are taking BYETTA.

This Patient Information includes the most important information you should know about using BYETTA. If you would like more information, talk with your healthcare provider. You can ask your healthcare provider or pharmacist for information about BYETTA that is written for health professionals.

- More information on BYETTA can be found at <http://www.BYETTA.com>.
- BYETTA Customer Service is available 24 hours a day at 1-800-868-1190.

What are the ingredients in BYETTA?

Active Ingredient: exenatide

Inactive Ingredients: metacresol, mannitol, glacial acetic acid, and sodium acetate trihydrate in water for injection.


Manufactured for Amylin Pharmaceuticals, Inc., San Diego, CA 92121
Marketed by Amylin Pharmaceuticals, Inc. and Eli Lilly and Company

Literature Revised February 2007

BYETTA is a registered trademark of Amylin Pharmaceuticals, Inc.

© 2007 Amylin Pharmaceuticals, Inc. All rights reserved.

823003-CC

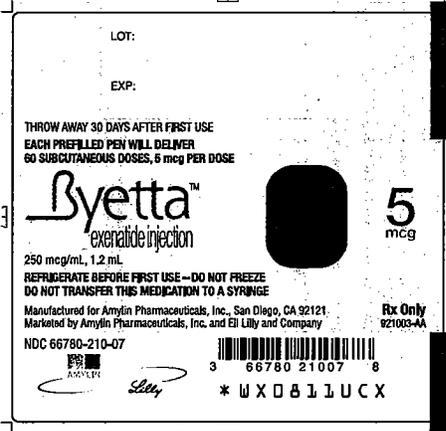

DIE ID	Die No.: 1910
	View: Printed Side Up

BKGD ID	D-1910-LB01
	Approved by: [Signature]
	Date: 07/26/04

LILLY APPROVALS	Graphics Operator:	Date:
	Proofreader:	Date:
	Label Editor or Label Editor Asst:	Date:
	Printing Quality Control:	Date:

VENDOR APPROVALS	Production Order Number:	
	Item Number:	Scanner Code:
	OK FOR PRODUCTION (copy only)	Client Services: Date:
	FINAL OK	Production Engineering: Date:

COLOR ID	Item Code: WX 0811 UCX	
	Colors:	
	BLACK	WX 0811 UCX
	0485 RED	WX 0811 UCX
	7459 BLUE	WX 0811 UCX
	3145 BLUE	WX 0811 UCX
	5085 ORANGE	WX 0811 UCX
	7472 GREEN	WX 0811 UCX
COATING	D-1910-LE01	

ENGINEER'S APPROVAL	D-1910-LE01
	Finishing Line No.: E1
	Approved by: [Signature]
	Date: 4/12/04
	Finishing Line No.:
	Approved by:
Date:	

LOT:
EXP:

THROW AWAY 30 DAYS AFTER FIRST USE
EACH PREFILLED PEN WILL DELIVER
60 SUBCUTANEOUS DOSES, 10 mcg PER DOSE

Byetta™
exenatide injection

250 mcg/mL, 2.4 mL

REFRIGERATE BEFORE FIRST USE—DO NOT FREEZE
DO NOT TRANSFER THIS MEDICATION TO A SYRINGE

Manufactured for Amylin Pharmaceuticals, Inc., San Diego, CA 92121
Marketed by Amylin Pharmaceuticals, Inc. and Eli Lilly and Company

Rx Only
921004-AA

NDC 66780-210-08

3 66780 21008 5

* W X 0 8 2 1 U C X

DIE ID	Die No.: 1910 [—] N/A View: Printed Side Up	BKGD ID	D-1910-LB01
			Approved by: [—] Date: 07/26/04
LILLY APPROVALS	Graphics Operator: _____ Date: _____	VENDOR APPROVALS	Production Order Number: _____
	Proofreader: _____ Date: _____		Item Number: _____ Scanner Code: _____
	Label Editor or Label Editor Asst: _____ Date: _____		OK FOR PRODUCTION (copy only) Client Services: _____ Date: _____
	Printing Quality Control: _____ Date: _____		FINAL OK Production Engineering: _____ Date: _____
COLOR ID	Item Code: WX 0821 UCX Colors: BLACK WX 0821 UCX 0485 RED WX 0821 UCX 7459 BLUE WX 0821 UCX 3145 BLUE WX 0821 UCX 7472 GREEN WX 0821 UCX COATING D-1910-LE01	ENGINEER'S APPROVAL	D-1910-LE01
			Finishing Line No.: E1
	Approved by: [—]		
	Date: 4/12/04		
	Finishing Line No.: _____		
	Approved by: _____		
	Date: _____		

PEN USER MANUAL

PATIENTS – READ ME FIRST

BYETTA®

exenatide injection

250 mcg/mL, 1.2 mL

5

mcg

Amylin Lilly (*logo*)

PV XXXX UCP

Pen User Manual

BYETTA®

exenatide injection

Prefilled Pen


Instructions for Use

Read and follow these instructions carefully.

Also, read the *Patient Information* insert inside your pen carton.

Pen Features

- A prefilled pen containing 60 subcutaneous doses of BYETTA for 30 days of use.
- The pen delivers a fixed 5 mcg dose.

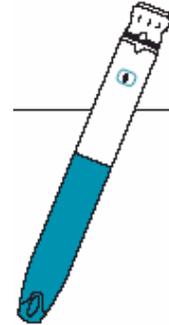

Important Notes

Read these instructions carefully before using your BYETTA Pen. Failure to follow these instructions completely may result, for example, in a wrong dose, a broken pen, or an infection.

- Check the label on your pen before each use to make sure you are using **your own** 5 mcg BYETTA Pen.
- **You must follow instructions in the New Pen Setup section for each new pen before its first use. The New Pen Setup is only done before each new pen is used for the first time. See Questions and Answers, number 1.**
- If any part of your pen appears broken or damaged, do not use the pen.
- This pen is not recommended for use by blind or visually impaired persons without the assistance of a person trained in the proper use of the product.
- **DO NOT TRANSFER THIS MEDICATION TO A SYRINGE.**
- Make sure the liquid in the BYETTA cartridge is clear, colorless, and free of particles. If not, do not use the pen.
- **Follow the instructions for sanitary injection technique recommended by your healthcare professional.**

Needles

- Pen needles are not included. Use 29 (thin), 30, or 31 (thinner) gauge disposable pen needles with your BYETTA Pen. Ask your healthcare professional which needle gauge and length is best for you.
- Use a new needle for each injection. Remove the needle after completing each injection. This will help prevent leakage of BYETTA, keep out air bubbles, reduce needle clogs, and minimize risk of infection.
- Do not share your pen or needles.
- Be sure the needle is completely attached to the pen before use. Do not push the injection button unless a needle is attached to the pen.
- Throw away used needles in a puncture-resistant container or as directed by your healthcare professional. Do not throw away the pen with a needle attached.
- Healthcare professionals or other caregivers should follow local or institutional policies regarding needle handling.

Storage

- Prior to first use, store your unused BYETTA Pen in the original carton in a refrigerator at 36°F to 46°F (2°C to 8°C).
- After first use, your BYETTA Pen can be kept at a temperature not to exceed 77°F (25°C).
- Do not freeze. Do not use BYETTA if it has been frozen. BYETTA should be protected from light.
- You can use your BYETTA Pen for up to 30 days after setting up a new pen for first use. **After 30 days, throw away the BYETTA Pen, even if it is not completely empty.** Mark the date when you first used your pen and the date 30 days later in the space provided in this Pen User Manual.
- When carrying the pen away from home, store the pen at a temperature between 36°F-77°F (2°C to 25°C) and keep dry.
- BYETTA should not be used after the expiration date printed on the label.
- Do not store the pen with the needle attached. If the needle is left on, BYETTA may leak from the pen and air bubbles may form in the cartridge.
- Keep your pen and needles out of the reach of children.

Cleaning

- If needed, wipe the outside of the pen with a clean, damp cloth.
- White particles may appear on the outside tip of the cartridge during normal use. You may remove them with an alcohol wipe or alcohol swab.

Questions and Answers

1. Do I need to do the New Pen Setup before every dose?

No. **The New Pen Setup is only done before each new pen is used for the first time.** The purpose of the setup is to check the flow of BYETTA from the tip of the needle. The small amount used in the New Pen Setup will not affect the 30-day supply of BYETTA. **If you repeat the New Pen Setup before each routine use, you will not receive 30 days of BYETTA from your pen.**

2. Why are there air bubbles in the cartridge?

A small air bubble is normal. It will not harm you or affect your dose. If the pen is stored with a needle attached, air bubbles may form in the cartridge. Do not store the pen with the needle attached.

3. What should I do if BYETTA does not come out of the needle tip during New Pen Setup?

Carefully replace the outer needle shield and remove the needle. Attach a new needle, and repeat the instructions in New Pen Setup. If liquid is seen (stream or several drops), setup is complete.

4. Why is it hard to push the injection button in all the way?

The injection button may be hard to push because no needle is attached, the needle is not correctly attached, or because the needle is clogged.

Step 1) Attach a new needle. Make sure the needle is on straight and screwed on all the way.

Step 2) Hold pen with needle pointing up and push the injection button in all the way. Several drops or a tiny stream of BYETTA should come from the needle tip.

5. Why do I see BYETTA leaking from my needle after I inject?

A single drop may remain after injection is complete. This is normal.

If you see more than one drop:

- You may not have received your full dose. Do not inject another dose. Consult with your healthcare professional about how to handle a partial dose.
- To prevent this, for your next dose, make sure to **firmly push and hold** the injection button in and **slowly count to 5** (also see Step 8 of the Inject the Dose section on the other side of this Pen User Manual).

6. How can I tell when the injection is complete?

The injection is complete when:

- you have firmly pushed the injection button in all the way until it stops **and**
- you have slowly counted to 5 while maintaining pressure on the injection button with the needle still in your skin **and**
- the  is in the center of the dose window.

7. Why can't I pull, turn, or push the dose knob?

Check the symbol in the dose window and follow the steps next to the matching symbol.

If  is in the dose window, pull the dose knob out until  appears.

If  is in the dose window and the dose knob won't turn, the cartridge in your BYETTA Pen may not have enough liquid to deliver a full dose. A small amount of BYETTA will always remain in the cartridge. If the cartridge contains a small amount or appears empty, obtain a new BYETTA Pen.

If  and part of the 5 are in the dose window and the dose knob can't be pushed in, the dose knob was not turned all the way. Continue turning until 5 clearly appears in the dose window.

If  is in the dose window and the dose knob won't turn, the injection button was not pushed in all the way and a complete dose was not delivered. Call your healthcare professional if you think you did not receive a complete dose. Follow these steps for your next injection:


Step 1) Hold the pen with needle up and firmly push the injection button in all the way until it stops. Continue applying pressure to injection button and slowly count to 5. Then turn the dose knob away from you (clockwise) until  appears in the dose window.

Step 2) If you cannot turn the dose knob, the needle may be clogged. Replace the needle and repeat Step 1 above.

Step 3) For your next dose, be sure to **firmly push and hold** the injection button in and **slowly count to 5** before removing needle from skin.

This Pen User Manual does not take the place of talking with your health-care professional about your medical condition or your treatment. If you are having problems using your BYETTA Pen, call toll free 800-868-1190.

New Pen Setup Read This before each new pen is used for the first time. Set up pen **only** at the start of its 30 days of use.




Wash hands prior to use.

Check pen label before each use to make sure it is your 5 mcg BYETTA Pen.

Pull off blue pen cap.

Check BYETTA in the cartridge. The liquid should be clear, colorless, and free of particles. If not, do not use.

A small air bubble in the cartridge is normal.




Remove paper tab from outer needle shield.

Push capped needle **straight** onto pen.

Screw needle on until secure.


Pull off outer needle shield. **Do not** throw away.

Pull off inner needle shield and throw away.



Check that  is in dose window.


If not, turn dose knob away from you (clockwise) **until it stops** and  is in dose window.



Pull dose knob out **until it stops** and  is in dose window.




Turn dose knob away from



With needle pointing up,

- **firmly push** injection button in all the way **until it stops** and
- **Keep holding injection button firmly** and
- **slowly count to 5.**

Watch for a stream or several drops. If none, repeat Steps C, D, and E up to three more times until a stream or several drops are



When  is in the center of dose window, pen is ready to reset. Turn dose knob away from you **until it stops** and  is in dose window.


Go to **Dial the Dose** section below.

Important: Do not repeat New Pen Setup before each

you **until it stops** and **5** is in dose window.

seen. If BYETTA still does not come from needle tip, see **Questions and Answers**, number 3.

routine use or you will not receive 30 days of BYETTA from your pen.

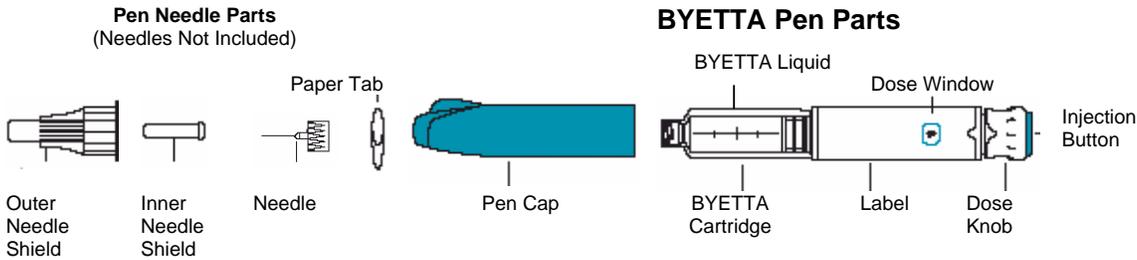


Dose Window Symbols:
 → ready to pull dose knob out
 + ready to turn to dose position
 5 ready to inject 5 mcg
 ↓ dose knob in and ready to reset

Routine Use Follow these instructions for each routine injection.


Attach the Needle

Check pen label before each use to make sure it is your 5 mcg BYETTA Pen. **Use a new needle for each injection.**




Wash hands prior to use. Pull off blue pen cap and check BYETTA in the cartridge. The liquid should be clear, colorless, and free of particles. If not, do not use.

A small air bubble will not harm you or affect your dose.




Remove paper tab from outer needle shield. Push capped needle **straight** onto pen. Screw needle on until secure.




Pull off outer needle shield. **Do not** throw away. Pull off inner needle shield and throw away. A small drop of liquid may appear. This is normal.

Dial the Dose



Check that → is in dose window.



Pull dose knob out **until it stops** and + is in



Turn dose knob away from you **until it stops** and 5 is


If not, turn dose knob away from you (clockwise) **until it stops** and  is in dose window.

dose window.

in dose window.


Note: If you cannot turn dose knob away from you to , see **Questions and Answers**, number 7.

Inject the Dose



Grip the pen firmly in your hand.

Insert needle into skin using injection technique recommended by your healthcare professional.

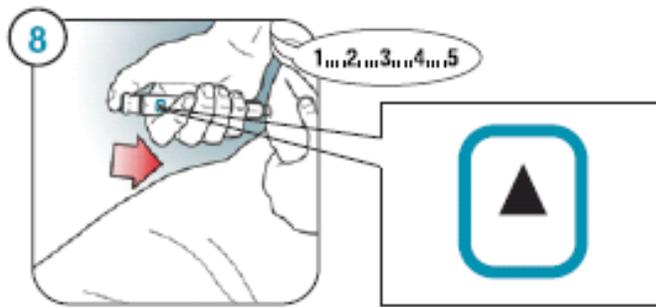


- Use thumb to **firmly push** injection button in all the way **until it stops and**
- **keep holding injection button firmly and**
- **slowly count to 5 to deliver full dose.**

Remove needle from skin.


Injection is complete when  is in the center of dose window.

If several drops of BYETTA are leaking from the needle, the injection button was not pushed in all the way. See **Questions and Answers**, number 5.



Reset the pen by turning dose knob away from you (clockwise) **until it stops** and  is in dose window.

Note: If you cannot turn dose knob or your pen leaks, your full dose has not been delivered. See **Questions and Answers**, numbers 5 and 7.



Carefully replace outer needle shield.

Unscrew needle and place in a puncture-resistant container.

Note: Remove needle after each injection.

Replace blue cap on pen before storage.

1st use date
____/____/____

Throw away 30 days after first use date,

OR

on expiration date printed on pen label, whichever date comes first.

Throw away date
____/____/____

For additional Information, call toll free 800-868-1190 or visit www.BYETTA.com

Manufactured for Amylin Pharmaceuticals, Inc.,

San Diego, CA 92121

Marketed by Amylin
Pharmaceuticals, Inc., and
Eli Lilly and Company
© 2006 Amylin
Pharmaceuticals, Inc., and Eli
Lilly and Company. All rights
reserved. BYETTA is a
registered trademark of Amylin
Pharmaceuticals, Inc.
Literature revised MONTH
YEAR

PV XXXX UCP

PEN USER MANUAL

PATIENTS – READ ME FIRST

BYETTA®

exenatide injection

250 mcg/mL, 2.4 mL

10

mcg

Amylin Lilly (*logo*)

PV XXXX UCP

Pen User Manual

BYETTA®

exenatide injection

Prefilled Pen


Instructions for Use

Read and follow these instructions carefully.

Also, read the *Patient Information* insert inside your pen carton.

Pen Features

- A prefilled pen containing 60 subcutaneous doses of BYETTA for 30 days of use.
- The pen delivers a fixed 10 mcg dose.

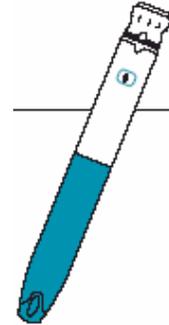

Important Notes

Read these instructions carefully before using your BYETTA Pen. Failure to follow these instructions completely may result, for example, in a wrong dose, a broken pen, or an infection.

- Check the label on your pen before each use to make sure you are using **your own** 10 mcg BYETTA Pen.
- **You must follow instructions in the New Pen Setup section for each new pen before its first use. The New Pen Setup is only done before each new pen is used for the first time. See Questions and Answers, number 1.**
- If any part of your pen appears broken or damaged, do not use the pen.
- This pen is not recommended for use by blind or visually impaired persons without the assistance of a person trained in the proper use of the product.
- **DO NOT TRANSFER THIS MEDICATION TO A SYRINGE.**
- Make sure the liquid in the BYETTA cartridge is clear, colorless, and free of particles. If not, do not use the pen.
- **Follow the instructions for sanitary injection technique recommended by your healthcare professional.**

Needles

- Pen needles are not included. Use 29 (thin), 30, or 31 (thinner) gauge disposable pen needles with your BYETTA Pen. Ask your healthcare professional which needle gauge and length is best for you.
- Use a new needle for each injection. Remove the needle after completing each injection. This will help prevent leakage of BYETTA, keep out air bubbles, reduce needle clogs, and minimize risk of infection.
- Do not share your pen or needles.
- Be sure the needle is completely attached to the pen before use. Do not push the injection button unless a needle is attached to the pen.
- Throw away used needles in a puncture-resistant container or as directed by your healthcare professional. Do not throw away the pen with a needle attached.
- Healthcare professionals or other caregivers should follow local or institutional policies regarding needle handling.

Storage

- Prior to first use, store your unused BYETTA Pen in the original carton in a refrigerator at 36°F to 46°F (2°C to 8°C).
- After first use, your BYETTA Pen can be kept at a temperature not to exceed 77°F (25°C).
- Do not freeze. Do not use BYETTA if it has been frozen. BYETTA should be protected from light.
- You can use your BYETTA Pen for up to 30 days after setting up a new pen for first use. **After 30 days, throw away the BYETTA Pen, even if it is not completely empty.** Mark the date when you first used your pen and the date 30 days later in the space provided in this Pen User Manual.
- When carrying the pen away from home, store the pen at a temperature between 36°F-77°F (2°C to 25°C) and keep dry.
- BYETTA should not be used after the expiration date printed on the label.
- Do not store the pen with the needle attached. If the needle is left on, BYETTA may leak from the pen and air bubbles may form in the cartridge.
- Keep your pen and needles out of the reach of children.

Cleaning

- If needed, wipe the outside of the pen with a clean, damp cloth.
- White particles may appear on the outside tip of the cartridge during normal use. You may remove them with an alcohol wipe or alcohol swab.

Questions and Answers

1. Do I need to do the New Pen Setup before every dose?

No. **The New Pen Setup is only done before each new pen is used for the first time.** The purpose of the setup is to check the flow of BYETTA from the tip of the needle. The small amount used in the New Pen Setup will not affect the 30-day supply of BYETTA. **If you repeat the New Pen Setup before each routine use, you will not receive 30 days of BYETTA from your pen.**

2. Why are there air bubbles in the cartridge?

A small air bubble is normal. It will not harm you or affect your dose. If the pen is stored with a needle attached, air bubbles may form in the cartridge. Do not store the pen with the needle attached.

3. What should I do if BYETTA does not come out of the needle tip during New Pen Setup?

Carefully replace the outer needle shield and remove the needle. Attach a new needle, and repeat the instructions in New Pen Setup. If liquid is seen (stream or several drops), setup is complete.

4. Why is it hard to push the injection button in all the way?

The injection button may be hard to push because no needle is attached, the needle is not correctly attached, or because the needle is clogged.

Step 1) Attach a new needle. Make sure the needle is on straight and screwed on all the way.

Step 2) Hold pen with needle pointing up and push the injection button in all the way. Several drops or a tiny stream of BYETTA should come from the needle tip.

5. Why do I see BYETTA leaking from my needle after I inject?

A single drop may remain after injection is complete. This is normal.

If you see more than one drop:

- You may not have received your full dose. Do not inject another dose. Consult with your healthcare professional about how to handle a partial dose.
- To prevent this, for your next dose, make sure to **firmly push and hold** the injection button in and **slowly count to 5** (also see Step 8 of the Inject the Dose section on the other side of this Pen User Manual).

6. How can I tell when the injection is complete?

The injection is complete when:

- you have firmly pushed the injection button in all the way until it stops **and**
- you have slowly counted to 5 while maintaining pressure on the injection button with the needle still in your skin **and**
- the  is in the center of the dose window.

7. Why can't I pull, turn, or push the dose knob?

Check the symbol in the dose window and follow the steps next to the matching symbol.

If  is in the dose window, pull the dose knob out until  appears.

If  is in the dose window and the dose knob won't turn, the cartridge in your BYETTA Pen may not have enough liquid to deliver a full dose. A small amount of BYETTA will always remain in the cartridge. If the cartridge contains a small amount or appears empty, obtain a new BYETTA Pen.

If  and part of the 10 are in the dose window and the dose knob can't be pushed in, the dose knob was not turned all the way. Continue turning until 10 clearly appears in the dose window.

If  is in the dose window and the dose knob won't turn, the injection button was not pushed in all the way and a complete dose was not delivered. Call your healthcare professional if you think you did not receive a complete dose. Follow these steps for your next injection:


Step 1) Hold the pen with needle up and firmly push the injection button in all the way until it stops. Continue applying pressure to injection button and slowly count to 5. Then turn the dose knob away from you (clockwise) until  appears in the dose window.

Step 2) If you cannot turn the dose knob, the needle may be clogged. Replace the needle and repeat Step 1 above.

Step 3) For your next dose, be sure to **firmly push and hold** the injection button in and **slowly count to 5** before removing needle from skin.

This Pen User Manual does not take the place of talking with your health-care professional about your medical condition or your treatment. If you are having problems using your BYETTA Pen, call toll free 800-868-1190.

New Pen Setup Read This before each new pen is used for the first time. Set up pen **only** at the start of its 30 days of use.




Wash hands prior to use.

Check pen label before each use to make sure it is your 10 mcg BYETTA Pen.

Pull off blue pen cap.

Check BYETTA in the cartridge. The liquid should be clear, colorless, and free of particles. If not, do not use.

A small air bubble in the cartridge is normal.




Remove paper tab from outer needle shield.

Push capped needle **straight** onto pen.

Screw needle on until secure.


Pull off outer needle shield. **Do not** throw away.

Pull off inner needle shield and throw away.




Check that  is in dose window.

If not, turn dose knob away from you (clockwise) **until it stops** and  is in dose window.




Pull dose knob out **until it stops** and  is in dose window.



With needle pointing up,

- **firmly push** injection button in all the way **until it stops** and
- **Keep holding injection button firmly** and
- **slowly count to 5.**

Watch for a stream or several drops. If none, repeat Steps C, D, and E up to three more times until a stream or several drops are



When  is in the center of dose window, pen is ready to reset. Turn dose knob away from you **until it stops** and  is in dose window.


Go to **Dial the Dose** section below.

Important: Do not repeat New Pen Setup before each

Turn dose knob away from you **until it stops** and **10** is in dose window.

seen. If BYETTA still does not come from needle tip, see **Questions and Answers**, number 3.

routine use or you will not receive 30 days of BYETTA from your pen.

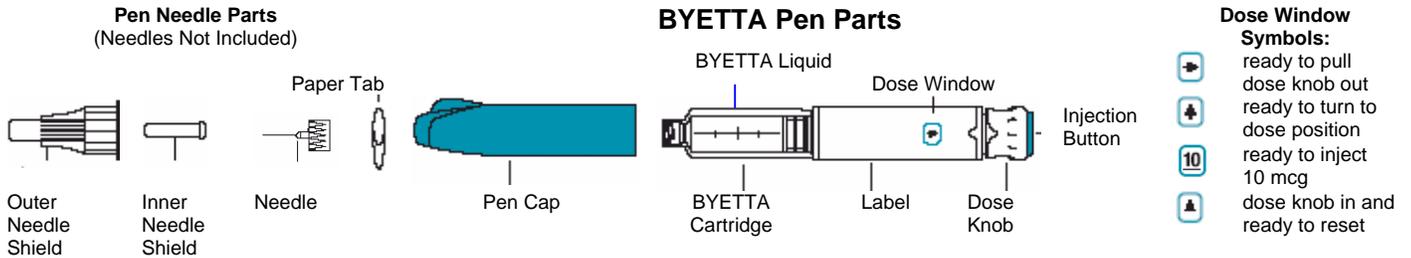


Routine Use

Follow these instructions for each routine injection.

Attach the Needle


Check pen label before each use to make sure it is your 10 mcg BYETTA Pen.

Use a new needle for each injection.




Wash hands prior to use.
Pull off blue pen cap and check BYETTA in the cartridge. The liquid should be clear, colorless, and free of particles. If not, do not use.

A small air bubble will not harm you or affect your dose.




Remove paper tab from outer needle shield.
Push capped needle **straight** onto pen.
Screw needle on until secure.




Pull off outer needle shield. **Do not** throw away.
Pull off inner needle shield and throw away.
A small drop of liquid may appear. This is normal.


Dial the Dose



Check that **10** is in dose



Pull dose knob out **until**



Turn dose knob away from

window.

If not, turn dose knob away from you (clockwise) **until it stops**


and  is in dose window.

it stops and  is in dose window.

you **until it stops** and  is in dose window.


Note: If you cannot turn dose knob away from you to , see **Questions and Answers**, number 7.

Inject the Dose



Grip the pen firmly in your hand.

Insert needle into skin using injection technique recommended by your healthcare professional.

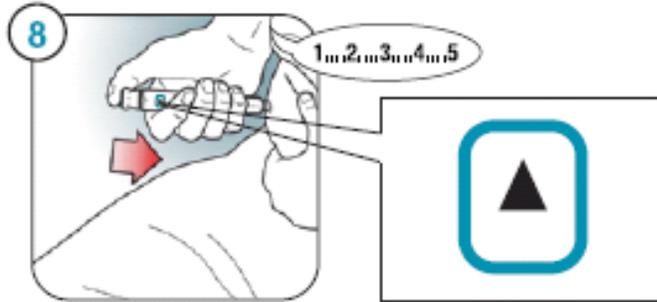


- Use thumb to **firmly push** injection button in all the way **until it stops** and
- **keep holding injection button firmly and**
- **slowly count to 5 to deliver full dose.**

Injection is complete when  is in the center of dose window.


If several drops of BYETTA are leaking from the needle, the injection button was not pushed in all the way. See **Questions and Answers**, number 5.

Remove needle from skin.



Reset the pen by turning dose knob away from you (clockwise) **until it stops** and  is in dose window.

Note: If you cannot turn dose knob or your pen leaks, your full dose has not been delivered. See **Questions and Answers**, numbers 5 and 7.



Carefully replace outer needle shield.

Unscrew needle and place in a puncture-resistant container.

Note: Remove needle after each injection.

Replace blue cap on pen before storage.

1st use date
____/____/____

Throw away 30 days after first use date,

OR

on expiration date printed on pen label, whichever date comes first.

Throw away date
____/____/____

For additional Information, call toll free 800-868-1190 or visit www.BYETTA.com

Manufactured for Amylin

Pharmaceuticals, Inc.,
San Diego, CA 92121

Marketed by Amylin
Pharmaceuticals, Inc., and
Eli Lilly and Company
© 2006 Amylin
Pharmaceuticals, Inc., and Eli
Lilly and Company. All rights
reserved. BYETTA is a
registered trademark of Amylin
Pharmaceuticals, Inc.
Literature revised MONTH
YEAR

PV XXXX UCP