

**CENTER FOR DRUG EVALUATION AND
RESEARCH**

APPLICATION NUMBER:

203324Orig1s000

LABELING

HIGHLIGHTS OF PRESCRIBING INFORMATION

These highlights do not include all the information needed to use PHOTREXA® VISCOUS and PHOTREXA® safely and effectively. See full prescribing information for PHOTREXA VISCOUS and PHOTREXA.

PHOTREXA VISCOUS (riboflavin 5'-phosphate in 20% dextran ophthalmic solution) 0.146% for topical ophthalmic use
PHOTREXA (riboflavin 5'-phosphate ophthalmic solution) 0.146% for topical ophthalmic use
For use with the KXL™ System
Initial U.S. Approval: 2016

INDICATIONS AND USAGE

PHOTREXA VISCOUS and PHOTREXA are photoenhancers indicated for use with the KXL System in corneal collagen cross-linking for the treatment of progressive keratoconus (1)

DOSAGE AND ADMINISTRATION

- Debride the epithelium using standard aseptic technique using topical anesthesia (2)
- Then instill 1 drop of PHOTREXA VISCOUS topically on the eye every 2 minutes for 30 minutes (2)
- After 30 minutes, examine the eye under slit lamp for presence of a yellow flare in the anterior chamber. If flare is not detected, instill 1 drop of PHOTREXA VISCOUS every 2 minutes for an additional 2 to 3 drops and recheck for yellow flare. Repeat as necessary (2).
- Once flare is observed, perform ultrasound pachymetry. If corneal thickness is less than 400 microns, instill 2 drops of PHOTREXA every 5 to 10 seconds until the corneal thickness increases to at least 400 microns (2).
- Irradiation should not be performed unless this 400 micron threshold is met and the yellow flare is seen (2).

- Irradiate the eye for 30 minutes at 3mW/cm² using the KXL System as per the instructions in the KXL manual. During irradiation, continue topical instillation of PHOTREXA VISCOUS onto the eye every 2 minutes for the 30 minute irradiation period (2).
- Refer to the *KXL Operator's manual* for specific device instructions (2).

DOSAGE FORMS AND STRENGTHS

- PHOTREXA VISCOUS in a 3 mL glass syringe containing sterile 1.46 mg/mL riboflavin 5'-phosphate in 20% dextran ophthalmic solution (3.1)
- PHOTREXA in a 3 mL glass syringe containing sterile 1.46 mg/mL riboflavin 5'-phosphate ophthalmic solution (3.2)

CONTRAINDICATIONS

None (4)

WARNINGS AND PRECAUTIONS

Ulcerative keratitis can occur. Monitor for resolution of epithelial defects (5)

ADVERSE REACTIONS

The most common ocular adverse reactions in any CXL-treated eye were corneal opacity (haze), punctate keratitis, corneal striae, corneal epithelium defect, eye pain, reduced visual acuity, and blurred vision (6.1).

To report SUSPECTED ADVERSE REACTIONS, contact Avedro at 1-800-xxx-xxxx or FDA at 1-800-FDA-1088 or www.fda.gov/medwatch.

See 17 for PATIENT COUNSELING INFORMATION

Revised: 4/2016

FULL PRESCRIBING INFORMATION: CONTENTS*

1. INDICATIONS AND USAGE
2. DOSAGE AND ADMINISTRATION
3. DOSAGE FORMS AND STRENGTHS
 - 3.1 PHOTREXA VISCOUS
 - 3.2 PHOTREXA
4. CONTRAINDICATIONS
5. WARNINGS AND PRECAUTIONS
6. ADVERSE REACTIONS
 - 6.1 Clinical Trial Experience
8. USE IN SPECIFIC POPULATIONS

- 8.1. Pregnancy
- 8.2. Lactation
- 8.4. Pediatric Use
- 8.5. Geriatric Use
11. DESCRIPTION
12. CLINICAL PHARMACOLOGY
 - 12.1. Mechanism of Action
13. NONCLINICAL TOXICOLOGY
 - 13.1. Carcinogenesis, Mutagenesis, Impairment of Fertility
14. CLINICAL STUDIES
16. HOW SUPPLIED/STORAGE AND HANDLING
17. PATIENT COUNSELING INFORMATION

*Sections or subsections omitted from the full prescribing information are not listed.

FULL PRESCRIBING INFORMATION

1. INDICATIONS AND USAGE

PHOTREXA® VISCOUS and PHOTREXA® are indicated for use in corneal collagen cross-linking in combination with the KXL™ System for the treatment of progressive keratoconus.

2. DOSAGE AND ADMINISTRATION

Using topical anesthesia, debride the epithelium to a diameter of approximately 9 mm using standard aseptic technique. Post epithelial debridement, instill 1 drop of Photrexa Viscous topically on the eye every 2 minutes for 30 minutes.

At the end of the 30 minute soaking period, examine the eye under the slit lamp for the presence of a yellow flare in the anterior chamber. If the yellow flare is not detected, instill 1 drop of Photrexa Viscous every 2 minutes for an additional 2 to 3 drops and recheck for the presence of a yellow flare. This process can be repeated as necessary.

Once the yellow flare is observed, perform ultrasound pachymetry. If corneal thickness is less than 400 microns, instill 2 drops of PHOTREXA every 5 to 10 seconds until the corneal thickness increases to at least 400 microns. Irradiation should not be performed unless this 400 micron threshold is met and the yellow flare is seen.

Irradiate the eye for 30 continuous minutes at $3\text{mW}/\text{cm}^2$ at a wavelength of 365 nm, centered over the cornea, using the KXL System as per the instructions in the KXL manual. During irradiation, continue topical instillation of PHOTREXA VISCOUS onto the eye every 2 minutes for the 30 minute irradiation period.

For topical ophthalmic use. Do not inject.

Single use PHOTREXA VISCOUS and PHOTREXA only. Discard syringe(s) after use.

PHOTREXA VISCOUS and PHOTREXA are for use with the KXL System only.

PLEASE REFER TO THE KXL OPERATOR'S MANUAL FOR SPECIFIC DEVICE INSTRUCTIONS.

3. DOSAGE FORMS AND STRENGTHS

3.1 PHOTREXA VISCOUS

PHOTREXA VISCOUS in a 3 mL glass syringe containing sterile 1.46 mg/mL riboflavin 5'-phosphate in 20% dextran ophthalmic solution for topical administration.

3.2 PHOTREXA

PHOTREXA in a 3 mL glass syringe containing sterile 1.46 mg/mL riboflavin 5'-phosphate ophthalmic solution for topical administration.

4. CONTRAINDICATIONS

None.

5. WARNINGS AND PRECAUTIONS

Ulcerative keratitis can occur. Monitor for resolution of epithelial defects. [*See Adverse Reactions (6)*].

6. ADVERSE REACTIONS

The following clinically significant adverse reactions are described elsewhere in the labeling:

Ulcerative keratitis [*Warnings and Precautions (5)*]

6.1 Clinical Trials Experience:

Because clinical trials are conducted under widely varying conditions, adverse reaction rates observed in the clinical trials of a drug cannot be directly compared to rates in the clinical trials of another drug and may not reflect the rates observed in practice.

The safety of the corneal collagen cross-linking procedure was evaluated in 3 randomized, parallel-group, open-label, sham-controlled trials; patients were followed up for 12 months. In each study, only one eye of subjects was designated as the study eye. Study eyes were randomized to receive one of the two study treatments (CXL or sham) at the baseline visit and were followed up at Day 1, Week 1, and Months 1, 3, 6, and 12. At Month 3 or later, sham study eyes and non-study eyes had the option of receiving CXL treatment, and were followed-up for 12 months from the time of receiving CXL treatment. Each CXL treated eye received a single course of CXL treatment only.

Safety data were obtained from 193 randomized CXL study eyes, 191 control eyes, and 319 nonrandomized CXL non-study eyes. Overall, 512 eyes in 364 patients received CXL treatment.

In progressive keratoconus subjects, the most common ocular adverse reactions in any CXL-treated eye were corneal opacity (haze), punctate keratitis, corneal striae, corneal epithelium defect, eye pain, reduced visual acuity, and blurred vision ([Table 1](#)).

Adverse events reported in non-study, non-randomized CXL treated were similar in terms of preferred terms and frequency to those seen in randomized study eyes.

The majority of adverse events reported resolved during the first month, while events such as corneal epithelium defect, corneal striae, punctate keratitis, photophobia, dry eye and eye pain, and decreased visual acuity took up to 6 months to resolve and corneal opacity or haze took up to 12 months to resolve. In 1-2% of patients, corneal epithelium defect, corneal edema, corneal opacity and corneal scar continued to be observed at 12 months.

Table 1: Most Common ($\geq 1\%$) Ocular Adverse Reactions in CXL-Treated Study Eye in the Pooled Randomized Safety Population – N (%)

Preferred Term	Progressive Keratoconus Studies		Other Clinical Experience	
	CXL Group (N=102) ¹	Control Group (N=103) ¹	CXL Group (N=91) ¹	Control Group (N=88) ¹
Anterior chamber cell	2 (2)	0	2 (2)	1 (1)
Anterior chamber flare	4 (4)	0	5 (6)	2 (2)
Asthenopia	1 (1)	1 (1)	2 (2)	0
Blepharitis	0	0	0	1 (1)
Corneal disorder	3 (3)	1 (1)	3 (3)	0
Corneal epithelium defect	24 (24)	1 (1)	26 (28)	3 (3)
Corneal oedema	3 (3)	0	3 (3)	0
Corneal opacity ²	65 (64)	9 (9)	65 (71)	8 (9)
Corneal striae	24 (24)	12 (12)	8 (9)	6 (7)
Corneal thinning	1 (1)	2 (2)	0	0
Diplopia	2 (2)	1 (1)	1 (1)	0
Dry eye	6 (6)	2 (2)	13 (14)	4 (5)
Eye complication associated with device	2 (2)	0	1 (1)	0
Eye discharge	2 (2)	1 (1)	0	0
Eye oedema	7 (7)	0	0	0
Eye pain	17 (17)	3 (3)	24 (26)	0
Eye pruritus	2 (2)	0	0	0
Eyelid oedema	5 (5)	0	5 (6)	1 (1)
Foreign body sensation in eyes	15 (15)	1 (1)	13 (14)	2 (2)
Glare	4 (4)	1 (1)	2 (2)	0
Halo vision	1 (1)	0	2 (2)	0
Keratitis	1 (1)	0	3 (3)	0
Lacrimation increased	5 (5)	0	9 (10)	1 (1)
Meibomian gland dysfunction	1 (1)	1 (1)	3 (3)	2 (2)
Ocular discomfort	0	0	8 (9)	0
Ocular hyperaemia	14 (14)	2 (2)	7 (8)	4 (5)
Photophobia	11 (11)	0	17 (19)	0

Preferred Term	Progressive Keratoconus Studies		Other Clinical Experience	
	CXL Group (N=102) ¹	Control Group (N=103) ¹	CXL Group (N=91) ¹	Control Group (N=88) ¹
Punctate keratitis	25 (25)	8 (8)	18 (20)	3 (3)
Vision blurred	16 (16)	2 (2)	15 (17)	4 (5)
Visual acuity reduced	10 (10)	9 (9)	10 (11)	1 (1)
Visual impairment	3 (3)	2 (2)	4 (4)	1 (1)
Vitreous detachment	2 (2)	0	0	0

1) Results are presented as the number (%) of subjects with an event from baseline to Month 3.

2) Almost all cases of corneal opacity were reported as haze.

Headache was reported in between 4 to 8% of treated patients.

8. USE IN SPECIFIC POPULATIONS

8.1. Pregnancy

Risk Summary

Animal development and reproduction studies have not been conducted with the PHOTREXA® VISCOUS/PHOTREXA®/KXL™ system. Since it is not known whether the corneal collagen cross-linking procedure can cause fetal harm or affect reproduction capacity, it should not be performed on pregnant women.

8.2. Lactation

Risk Summary

There are no data on the presence of PHOTREXA VISCOUS or PHOTREXA in human milk, the effects on the breastfed infant, or the effects on milk production. The developmental and health benefits of breastfeeding should be considered, along with the mother's clinical need for the PHOTREXA/KXL corneal collagen cross-linking procedure and any potential adverse effects on the breastfed child from the PHOTREXA/KXL corneal collagen cross-linking procedure or from the underlying maternal condition.

8.4. Pediatric Use

The safety and effectiveness of corneal collagen cross-linking has not been established in pediatric patients below the age of 14.

8.5. Geriatric Use

No subjects enrolled in the clinical studies were 65 years of age or older.

11. DESCRIPTION

PHOTREXA VISCOUS (riboflavin 5'-phosphate in 20% dextran ophthalmic solution) 0.146% and PHOTREXA (riboflavin 5'-phosphate ophthalmic solution) 0.146% are intended for topical ophthalmic administration as part of corneal collagen cross-linking with the KXL System.


PHOTREXA VISCOUS and PHOTREXA are supplied as:

- PHOTREXA VISCOUS in a 3 mL glass syringe containing sterile 1.46 mg/mL riboflavin 5'-phosphate in 20% dextran ophthalmic solution for topical administration.
- PHOTREXA in a 3 mL glass syringe containing sterile 1.46 mg/mL riboflavin 5'-phosphate ophthalmic solution for topical administration.

PHOTREXA VISCOUS (riboflavin 5'-phosphate in 20% dextran ophthalmic solution) 0.146% is a yellow sterile buffered viscous solution containing 1.46 mg/mL riboflavin 5'-phosphate and 20% dextran 500. The pH of the solution is approximately 7.1 and the osmolality is 301-339 mOsm/kg. Each 1 mL of solution contains 1.53 mg of riboflavin 5'-phosphate sodium (equivalent to 1.20 mg riboflavin). Riboflavin 5'-phosphate sodium USP is a mixture of the sodium salts of riboflavin, riboflavin monophosphates, and riboflavin diphosphates. The inactive ingredients are dibasic sodium phosphate, dextran, monobasic sodium phosphate, sodium chloride, and water for injection.

PHOTREXA (riboflavin 5'-phosphate ophthalmic solution) 0.146% is a yellow sterile buffered solution containing 1.46 mg/mL riboflavin 5'-phosphate. The pH of the solution is approximately 7.1 and the osmolality is 157-177 mOsm/kg. Each 1 mL of solution contains 1.53 mg of riboflavin 5'-phosphate sodium (equivalent to 1.20 mg riboflavin). Riboflavin 5'-phosphate sodium USP is a mixture of the sodium salts of riboflavin, riboflavin monophosphates, and riboflavin diphosphates. The inactive ingredients are dibasic sodium phosphate, monobasic sodium phosphate, sodium chloride, and water for injection.

The chemical formula for riboflavin 5'-phosphate sodium (Vitamin B2) is $C_{17}H_{20}N_4NaO_9P$ with a molecular mass of 478.33 g/mol.

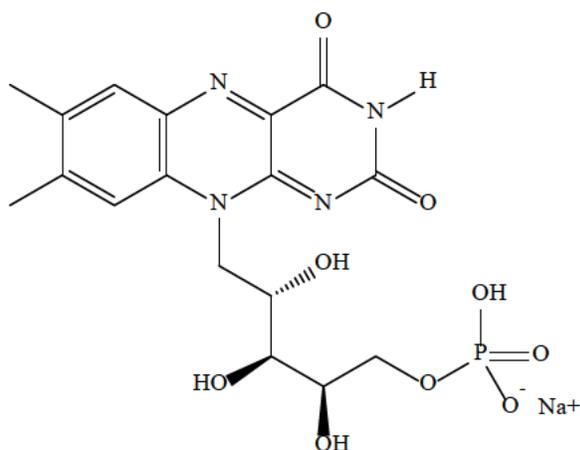

Please refer to the KXL System Operator's Manual for a specific device description and instructions.

12. CLINICAL PHARMACOLOGY

12.1. Mechanism of Action

Riboflavin 5'-phosphate sodium (Vitamin B2) is the precursor of two coenzymes, flavin adenine dinucleotide and flavin mononucleotide, which catalyze oxidation/reduction reactions involved in a number of metabolic pathways.

Under the conditions used for corneal collagen cross-linking, riboflavin 5'-phosphate functions as a photoenhancer and generates singlet oxygen which is responsible for the cross-linking.

13. NONCLINICAL TOXICOLOGY

13.1. Carcinogenesis, Mutagenesis, Impairment of Fertility

Animal studies have not been conducted to determine the carcinogenic potential of photoexcited riboflavin. Photoexcited riboflavin has been shown to be genotoxic in the Ames Salmonella reverse mutation assay and in the SOS/umu test system.

The genotoxicity of riboflavin, in the absence of photoexcitation has been examined in vitro in bacterial reverse mutation assays, sister chromatid exchange assay, chromosomal aberration assays and in vivo in a mouse micronucleus study. The overall weight of evidence indicates that riboflavin, in the absence of photoexcitation, is not genotoxic.


Animal studies to determine the effects of the PHOTREXA/KXL corneal collagen cross-linking procedure on fertility were not conducted.

14. CLINICAL STUDIES

Three prospective, randomized, parallel-group, open-label, sham-controlled trials were conducted to evaluate the safety and effectiveness of riboflavin ophthalmic solution/UVA irradiation for performing corneal collagen cross-linking. These trials were sham-controlled for the first 3 months and had a total duration of 12 months for safety and efficacy evaluations. Study 1 enrolled 58 patients with progressive keratoconus. Study 2 enrolled 147 patients with progressive keratoconus. In each study, patients had one eye designated as the study eye and were randomized to receive one of two study treatments (CXL or sham) in their study eye at the baseline visit. The patients were evaluated at Day 1, Week 1, and Months 1, 3, 6, and 12. At Month 3 or later, patients had the option of receiving CXL treatment in both the sham study eyes and non-study eyes and were followed-up for 12 months from the time of receiving CXL treatment. Approximately 56% and 89% of the sham study eyes in patients with progressive keratoconus received CXL treatment by Month 3 and Month 6, respectively. The average age of keratoconus patients was 33 years. The average baseline K_{max} value was 61 diopters.

In each study, the maximum corneal curvature (K_{\max}) was assessed at baseline, Months 1, 3, and 12. The CXL-treated eyes showed increasing improvement in K_{\max} from Month 3 through Month 12 (Figure 1). Progressive keratoconus patients had an average K_{\max} reduction of 1.4 diopter in Study 1 and 1.7 diopter in Study 2 at Month 12 in the CXL-treated eyes while the sham eyes had an average increase of 0.5 diopter in Study 1 and 0.6 diopter in Study 2 at Month 12; the difference (95% CI) between the CXL and sham groups in the mean change from baseline K_{\max} were -1.9 (-3.4, -0.3) diopters in Study 1 and -2.3 (-3.5, -1.0) diopters in Study 2.

Figure 1: Mean (SD) (Diopter) Baseline Kmax and Change from Baseline Kmax

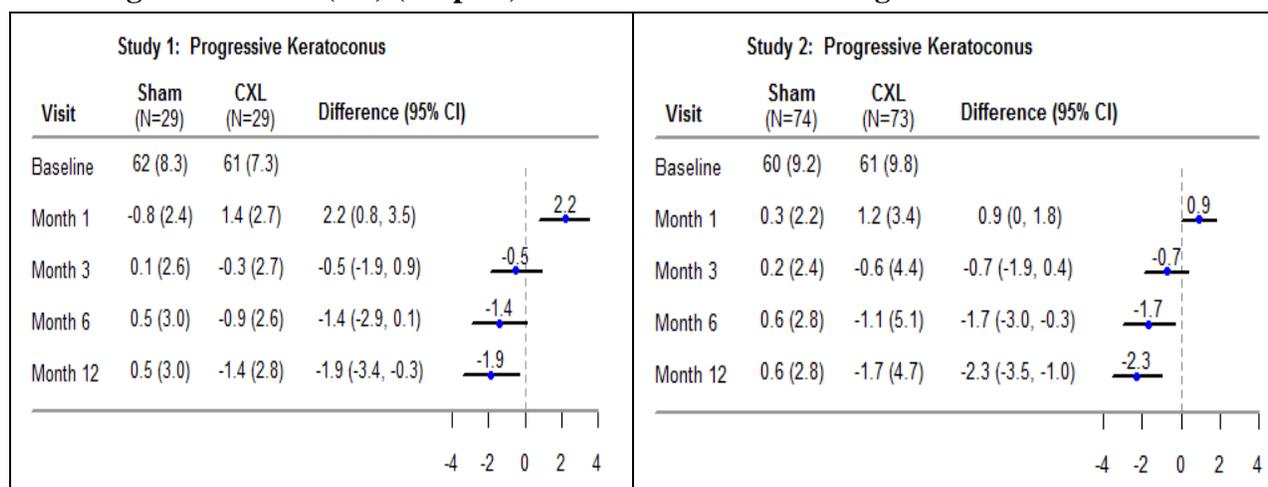

Post-baseline missing data were imputed using last available K_{\max} value. For the sham study eyes that received CXL treatment after baseline, the last K_{\max} measurement recorded prior to receiving CXL treatment was used in the analysis for later time points.

16. HOW SUPPLIED/STORAGE AND HANDLING

PHOTREXA[®] VISCOUS and PHOTREXA[®] are provided in a bulk pack of 10 (ten), single-use foil pouches. Each foil pouch contains a 3 mL glass syringe of PHOTREXA VISCOUS or PHOTREXA contained within a Tyvek[®] pouch.

The entire bulk pack should be stored at 15°-25°C (59°-77°F) and care should be taken to minimize exposure of the syringe to light once removed from its protective packaging. Discard syringe after use.

For topical ophthalmic use.

PHOTREXA VISCOUS and PHOTREXA should be used with the KXL System only.

17. PATIENT COUNSELING INFORMATION

- Patients should be advised not to rub their eyes for the first five days after their procedure.

- Patients may be sensitive to light and have a foreign body sensation. Patients should be advised that there may be discomfort in the treated eye and that sunglasses may help with light sensitivity.
- If patients experience severe pain in the eye or any sudden decrease in their vision, they should be advised to contact their physician immediately.
- If the bandage contact lens that was placed on the patient's eye on the day of treatment falls out or becomes dislodged, the patient should be advised not to replace it and to contact their physician immediately.

PHOTREXA® VISCOUS (riboflavin 5'-phosphate in 20% dextran ophthalmic solution) 0.146%, PHOTREXA® (riboflavin 5'-phosphate ophthalmic solution) 0.146% and the KXL™ System are marketed by: Avedro, 230 Third Avenue, Waltham, MA, 02451.

Version:

April 2016



Photrexa® Viscous Syringe Label

NDC: 25357-022-01 R_x Only
Photrexa® Viscous (riboflavin 5'-phosphate in
20% dextran ophthalmic solution) 0.146%
Lot: XXXXXXXX
Single-Patient Use Only, Sterile EXP: XX/XXXX
Mfg. for Avedro Inc. RM-XXXX, Rev.XXX

Photrexa® Viscous Tyvek® Pouch Label

NDC: 25357-022-01 R_x Only
Photrexa® Viscous (riboflavin 5'-phosphate in 20%
dextran ophthalmic solution) 0.146%
Pouch contains: Each Tyvek® pouch contains a 3 mL glass
syringe of Photrexa Viscous
Active ingredients: 1.46 mg/mL riboflavin-5'-phosphate
Inactive ingredients: 20% dextran 500, sodium chloride,
sodium phosphates (monobasic & dibasic), sterile water for
injection
For Single-Patient Use Only; For Ophthalmic Use 
25357-022-01-yy-yy
Storage: Store at 15°-25°C (59°-77°F); Protect from light
For Use with KXL® System; Lot: XXXXXXXX
Use immediately upon opening package EXP: XX/XXXX
Please see full prescribing information RM-XXXX, Rev.XXX
Mfg. for Avedro Inc. Waltham, MA 02451

Photrexa® Viscous Foil Pouch Label

NDC: 25357-022-01 R_x Only
Photrexa® Viscous (riboflavin 5'-phosphate in 20%
dextran ophthalmic solution) 0.146%
Pouch contains: Each foil pouch contains a 3 mL glass
syringe of Photrexa Viscous contained within a Tyvek®
pouch
Active ingredients: 1.46 mg/mL riboflavin-5'-phosphate
Inactive ingredients: 20% dextran 500, sodium chloride, sodium
phosphates (monobasic & dibasic), sterile water for injection
For Single-Patient Use Only; For Ophthalmic Use; 
25357-022-01-yy-yy
For Use with KXL® System;
Storage: Store at 15°-25°C (59°-77°F); Protect from Light
Use immediately upon opening package Lot: XXXXXXXX
Please see full prescribing information EXP: XX/XXXX
Mfg. for Avedro Inc. Waltham, MA 02451 RM-XXXX, Rev.XXX

Photrexa® Syringe Label

NDC: 25357-023-01

R_x Only

Photrexa® (riboflavin 5'-phosphate ophthalmic solution) 0.146 %

Lot: XXXXXXXX

Single-Patient Use Only, Sterile

EXP: XX/XXXX

Mfg. for Avedro Inc.

RM-XXXX, Rev.XXX

Photrexa® Tyvek® Pouch Label

NDC: 25357-023-01

R_x Only

Photrexa® (riboflavin 5'-phosphate ophthalmic solution) 0.146%

Pouch contains: Each Tyvek® pouch contains a 3 mL glass syringe of Photrexa

Active ingredients: 1.46 mg/mL riboflavin-5'-phosphate
Inactive ingredients: sodium chloride, sodium phosphates (monobasic & dibasic), sterile water for injection



For Single-Patient Use Only; For Ophthalmic Use
Storage: Store at 15°-25°C (59°-77°F); Protect from light

For Use with KXL® System;

Use immediately upon opening package

Lot: XXXXXXXX

Please see full prescribing information

EXP: XX/XXXX

Mfg. for Avedro Inc. Waltham, MA 02451

RM-XXXX, Rev.XXX

Photrexa® Foil Pouch Label

NDC: 25357-023-01

R_x Only

Photrexa® (riboflavin 5'-phosphate ophthalmic solution) 0.146%

Pouch contains: Each foil pouch contains a 3 mL glass syringe of Photrexa contained within a Tyvek® pouch

Active ingredients: 1.46 mg/mL riboflavin-5'-phosphate
Inactive ingredients: sodium chloride, sodium phosphates (monobasic & dibasic), sterile water for injection

For Single-Patient Use Only; For Ophthalmic Use;
For Use with KXL® System;
Storage: Store at 15°-25°C (59°-77°F); Protect from Light



Use immediately upon opening package

Please see full prescribing information

Lot: XXXXXXXX

EXP: XX/XXXX

Mfg. for Avedro Inc. Waltham, MA 02451

RM-XXXX, Rev.XXX

Avedro, Inc.
KXL™ System

Operator's Manual

ML-00006
Copyright 2015
Printed in U.S.A.

Revision H
All Rights Reserved

Patents, Trademarks, Copyrights

The KXL System may be covered by one or more patent applications issued or pending in the United States and worldwide.

“KXL” and the Avedro logo design are registered trademarks or trademarks of Avedro, Inc. All software and documentation is subject to Avedro, Inc. copyrights. All rights reserved 2015.

Microsoft and Windows are registered trademarks and trademarks, respectively, of Microsoft Corporation. Any other trademarks or service marks contained within this manual are the property of their respective owners.

CAUTION: Federal law restricts this device to sale by or on the order of a physician

For more information, contact:



Avedro, Inc.
230 Third Avenue
Waltham, MA 02451
+1-781-768-3400

Table of Contents

Chapter:

1	Foreword.....	1-1
1.1	Intended Use of Manual.....	1-1
1.2	Intended Use / Indications for Use.....	1-1
1.3	Confidentiality Disclaimer.....	1-1
1.4	Reproduction Disclaimer.....	1-1
1.5	User Operation Assistance Statement.....	1-1
1.6	Contraindications, Warnings and Cautions.....	1-1
	1.6.1 Contraindications.....	1-1
	1.6.2 Warnings.....	1-1
	1.6.3 Electrical Safety Warnings.....	1-1
	Radiation Safety Warnings.....	1-3
1.7	Patient Safety.....	1-3
1.8	Additional Safety Considerations.....	1-3
1.9	FCC Compliance Notice.....	1-4
2	Introduction.....	2-1
2.1	System Overview.....	2-1
	2.1.1 Major Components.....	2-2
3	System Operation.....	3-1
3.1	Charging the KXL Battery.....	3-1
3.2	Touchpad/Keyboard Use.....	3-1
3.3	UV Dose.....	3-3
3.4	Preparing the System.....	3-3
3.5	Important Steps before Turning on the System.....	3-3
3.6	Powering Up the System.....	3-3
3.7	Confirm Riboflavin Induction Period.....	3-4
3.8	Confirm UV Treatment.....	3-5
	3.8.1 Confirm UV Dose.....	3-5
3.9	Starting Treatment.....	3-6
	3.9.1 Single-use disposables.....	3-7
	3.9.2 Multi-use disposables.....	3-8
	3.9.3 Sync Alignment Remote.....	3-9
3.10	Preparing the Patient.....	3-11
3.11	Administration of Photrexa Viscous.....	3-11
3.12	Confirm Riboflavin Absorption.....	3-11
3.13	Confirm Corneal Thickness.....	3-12
3.14	Alignment of the Device.....	3-12
3.15	Initiating Treatment.....	3-13
3.16	Monitoring Treatment.....	3-14
3.17	Stopping a Treatment.....	3-15

3.18	Treatment Complete.....	3-15
3.19	Pausing or Canceling a Treatment	3-17
3.20	Powering Down the System.....	3-19
3.21	Using the Device Settings Menu.....	3-20
3.21.1	Advanced Settings.....	3-21
3.21.2	Editing System Language.....	3-22
3.21.3	Editing Alignment Crosshairs Intensity	3-22
3.21.4	Editing System Volume	3-22
3.21.5	Copying Treatment Data to USB	3-23
3.21.6	Confirming Treatment Settings.....	3-25
4	Maintenance / Service.....	4-1
4.1	Installation Policy	4-1
4.2	Customer Maintenance	4-1
4.3	Warranty Information	4-1
4.4	Service Contract Information.....	4-1
4.5	Trouble-shooting.....	4-2
4.6	Directions for Sterilization or Disinfection.....	4-3
4.7	Cleaning the System	4-3
4.8	Cleaning the Aperture	4-3
4.9	Articulating Arm Adjustment	4-3
4.10	Moving the System	4-4
4.11	Storing the System	4-4
4.12	Software	4-4
4.13	Identifying Risks Associated with Disposing of Waste Products.....	4-5
4.14	Performing a Visible Check.....	4-5
5	Equipment Classification	5-1
5.1	Essential Performance.....	5-1
5.2	Equipment Classification	5-1
5.3	EMC Guidance.....	5-2
	Separation distance according to frequency of transmitter (m)	5-5
5.4	RF Transmitters	5-5
5.4.1	RFID reader:.....	5-5
5.4.2	Wireless remote control:	5-6
6	Symbol Library	6-1
7	Specifications	7-1

Table of Figures

Figure 2-1. Overview Illustration of System	2-2
Figure 2-2. System Illustrations with Callouts	2-3
Figure 2-3. Wireless Remote	2-3
Figure 2-4. KXL Label	2-4
Figure 2-5. UV emitting Label	2-4
Figure 2-6. Alignment Laser Classification Label	2-4
Figure 3-1. Power Switch	3-4
Figure 3-2. Startup Screen	3-4
Figure 3-3. Induction Period Screen	3-5
Figure 3-4. UV Energy Dose	3-6
Figure 3-5. Confirm Treatment Parameters Screen	3-6
Figure 3-6. Reading Activation Card	3-7
Figure 3-7. Treatments Remaining	3-8
Figure 3-8. Final Treatment	3-8
Figure 3-9. No Treatments Remaining	3-9
Figure 3-10. Remote Synch Status	3-9
Figure 3-11. Prepare Patient Screen	3-11
Figure 3-12. Align Crosshairs during induction	3-12
Figure 3-13. Remote Functions.....	3-13
Figure 3-14. Red Crosshairs X & Y Axes, Red Crosshairs Z Axis Alignment	3-13
Figure 3-15. Induction Complete	3-14
Figure 3-16. Treatment Screen	3-15
Figure 3-17. Treatment Paused Screen.....	3-15
Figure 3-18. Treatment Complete Screen	3-16
Figure 3-19. Confirm Cancel Session Screen	3-17
Figure 3-20. Confirm Cancel Partial Treatment.....	3-17
Figure 3-21. Partial Treatment Information.....	3-18
Figure 3-22. Power Off.....	3-18
Figure 3-23. Power Off Position	3-20
Figure 3-24. KXL System Plug	3-20
Figure 3-25. Device Settings Menu	3-21
Figure 3-26. Edit System Language	3-22
Figure 3-27. Edit Alignment Crosshairs Intensity	3-22
Figure 3-28. Edit Volume	3-23
Figure 3-29. Data Transfer to USB	3-23
Figure 3-30. Edit Default Treatment Parameters	3-25
Figure 4-1. Remote Lost Sync	4-2
Figure 4-2 Moving System Configuration	4-4
Table 5-1	5-2
Table 5-2	5-3
Table 5-3	5-4
Table 5-4	5-5
Table 5-5	5-6

1 Foreword

1.1 Intended Use of Manual

This manual is designed to serve the operators of the Avedro, Inc. KXL System. All operating instructions, product illustrations, screen graphics, troubleshooting/error messages, and other relevant information are contained in this manual. It is the operator's responsibility to ensure that all safety instructions in this manual are applied strictly.

1.2 Intended Use / Indications for Use

The KXL™ System is indicated for use with PHOTREXA (riboflavin 5'-phosphate ophthalmic solution) and PHOTREXA VISCOUS (riboflavin 5'-phosphate in 20% dextran ophthalmic solution) in corneal collagen cross-linking for the treatment of progressive keratoconus.

1.3 Confidentiality Disclaimer

All patient data appearing in this document, including the sample screen graphics, are fictitious and representative only. No patient's confidentiality has been violated, with or without permission.

1.4 Reproduction Disclaimer

Neither this manual nor any part of it may be reproduced, photocopied, or electronically transmitted in any way without the advanced written permission of Avedro, Inc.

1.5 User Operation Assistance Statement

Should you experience any difficulty in running your KXL System, please contact your local Avedro authorized representative.

1.6 Contraindications, Warnings and Cautions

1.6.1 Contraindications

None.

1.6.2 Warnings

Ulcerative keratitis can occur. Epithelial defects should be monitored until resolution.

1.6.3 Electrical Safety Warnings

This equipment requires special precautions regarding electromagnetic compatibility (EMC). Installation and use should be carried out according to the EMC information provided in this manual.

Portable and mobile RF communications equipment can affect medical electrical equipment such as the Avedro KXL System.

For Equipment Classifications please refer to Chapter 5.0 Equipment Classifications



WARNING: To avoid the risk of shock this equipment must only be connected to a supply mains with protective earth.

Even with the power cord removed, there is the potential for an electrical shock from the 12VDC internal power source.

The system is designed for continuous operation using the external connector or its internal rechargeable battery.



WARNING: This equipment is operated with hazardous voltages that can shock, burn, or cause death. To reduce the possibility of electrical shock, and inadvertent UVA exposure do not remove any fixed panels. Ensure that all service to the system, beyond what is described in this manual, including to the rechargeable battery, is performed only by qualified Avedro service personnel.



WARNING: Remove the wall plug and turn off the power switch before servicing or cleaning (disinfecting) the equipment.

Never pull cords to remove the power cord from the outlet. Grasp the power cord plug and pull it from the outlet to disconnect.



WARNING: Do not operate the equipment with a damaged power cord.



WARNING: Position the power cord so that it cannot be tripped over, walked on, rolled over, crimped, bent, pinched, or accidentally pulled from the wall outlet.



WARNING: Do not use the instrument near water and be careful not to spill liquids on any part of it.



WARNING: The USB port can only be used when the system is not in treatment mode, do not connect to the USB during treatment.



WARNING: Do not operate the KXL System in the presence of flammable mixtures or anesthetics.



WARNING: The remote contains replaceable batteries; if system is not going to be used for an extended period of time remove the batteries.



WARNING: Do not use adjacent to or stack with other equipment; if it is used adjacent to or stacked with other equipment, verify that the equipment behaves normally as intended.



WARNING: No modification of this equipment is allowed.



WARNING: MR Unsafe – Keep away from magnetic resonance imaging equipment.

Radiation Safety Warnings



WARNING: Never look directly into the UV light beam nor direct the beam towards a person except for therapeutic purposes.



WARNING: Always wear UVA protective goggles when the KXL system is turned on.



WARNING: use only laser grade instruments in order to prevent reflected UV radiation from smooth metallic surfaces.

1.7 Patient Safety

- The treatment should take place in a quiet atmosphere in order not to distract the attention of the patient. The patient should lie on a table or patient's chair. The patient's head should rest comfortably in a headrest. It is imperative that the table or patient's chair or the system not be moved during the treatment procedure.



CAUTION: The KXL System is a medical device. It may be operated, therefore, only in health care facilities or medical areas under the supervision of medically trained personnel.

1.8 Additional Safety Considerations

- Any modification of the system's external light beam by means of optical elements is strictly prohibited.
- Plastic instrumentation such as speculums or eye shields may be damaged when impacted by the UV beam, possibly resulting in product degradation.

1.9 FCC Compliance Notice

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an electrical outlet on a circuit different from that to which the receiver is connected.
- Consult Avedro Customer Service for help.

Properly shielded and grounded cables and connectors must be used in order to meet FCC emission limits. Proper cables and connectors are available from Avedro. Avedro is not responsible for any radio or television interference caused by unauthorized changes or modifications to this equipment. Unauthorized changes or modifications could void the user's authority to operate the equipment.

2 Introduction

2.1 System Overview

The KXL System is an electronic medical device which delivers ultraviolet light (365 nm wavelength) in a circular pattern onto the cornea after riboflavin phosphates ophthalmic solution (Photrexa Viscous and/or Photrexa) has been applied. Irradiating the riboflavin phosphates ophthalmic solution creates singlet oxygen, which forms intermolecular bonds in corneal collagen. UV flux and irradiation time (that is, fluence) at the cornea are controlled by an onboard computer system.

The *Optics Head* houses the UVA irradiation mechanism. The LED emits continuous UVA radiation at a wavelength of 365 nm at an intensity of 3 mW/cm².

A fixed aperture mounted in the UVA irradiation beam path is used to produce a circular area of irradiation at the treatment plane with a diameter of 9.5 mm. Alignment lasers are used to aid the user in focusing the beam on the patient's cornea. Fine alignment of the UV beam through observation of the alignment lasers is controlled by the user through a wireless remote.

The KXL is a portable system with an articulating arm to allow movement of the system for alignment of the UV beam to the patient's cornea. An internal battery powers the system; the battery is recharged by a system internal charger from any standard AC outlet. The treatment parameters (Riboflavin Induction Period, Total UV Energy and UV Power) are confirmed through the user interface touch screen computer.

The KXL System is used in conjunction with Photrexa Viscous and Photrexa and an RFID activation card.

2.1.1 Major Components

The major components of the KXL System include the following:

- **Optics Head with UV source**
- **KXL console with user interface**
- **Wireless remote control** (with replaceable batteries)



Figure 2-1. Overview Illustration of System

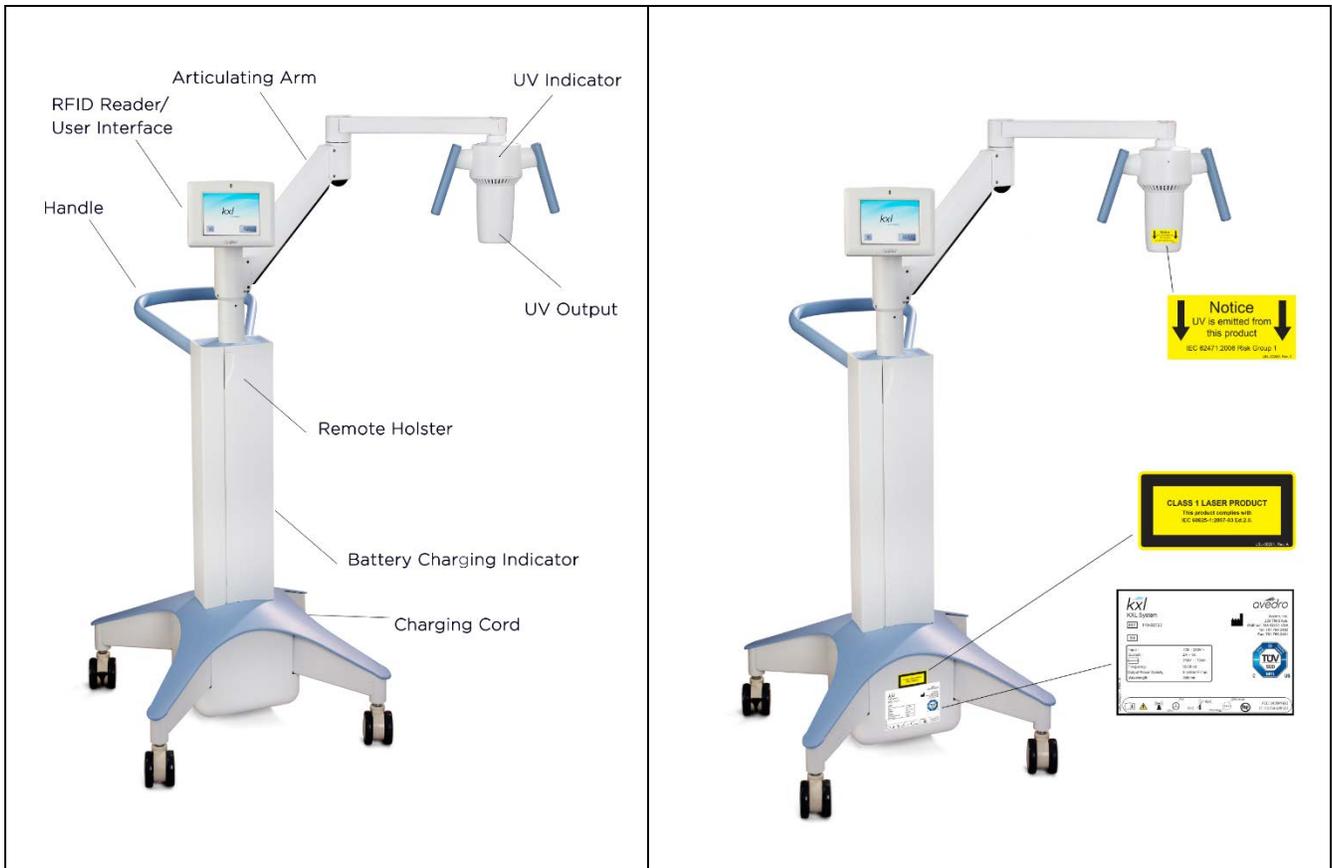


Figure 2-2. System Illustrations with Callouts



Figure 2-3. Wireless Remote

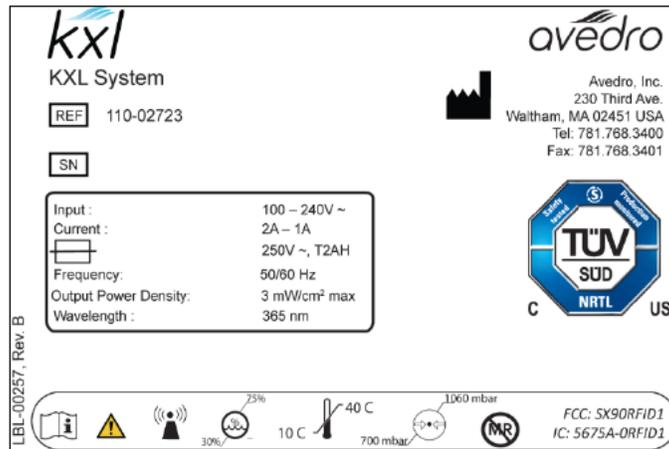


Figure 2-4. KXL Label



Figure 2-5. UV emitting Label



Figure 2-6. Alignment Laser Classification Label

3 System Operation

3.1 Charging the KXL Battery

NOTE: Prior to initial use, the internal battery pack of the KXL must be charged overnight.

- In order to maintain battery charge, it is recommended that the KXL be connected to a grounded supply mains at the end of each business day or when not in use.
- The charging status of the battery is identified by the color of the light located on the column of the KXL.
 - Orange – low, charging
 - Yellow – charging
 - Green – fully charged

NOTE: if the battery does not appear to be charging or retaining its charge, please contact your local Avedro Service Representative.

NOTE: the KXL battery should last for 16 hours during normal operation. The system software will notify the user when the battery needs to be charged. The KXL system prohibits a treatment if there is insufficient battery power to perform a treatment. (See Chapter 4 Maintenance for more information on troubleshooting battery problems.)

3.2 Touchpad/Keyboard Use

The table below identifies and describes important touchpad keys and icons unique to KXL System operation. Chapter 2 identifies and describes the system's major components.

Touchpad Key	Icon	Description/Function
Power Off button (Initial screen)		Turns OFF electric power to the internal computer.
Start New Treatment button (Initial screen)		Starts a new clinical treatment protocol.
UP arrow (various Clinical Protocol screens)		Increases the value of the current field.
DOWN arrow (various Clinical Protocol screens)		Decreases the value of the current field.

Touchpad Key	Icon	Description/Function
X button (various Device Settings screens)		Cancels all the entries on a particular screen and returns to the previous screen.
Checkmark button (various Clinical Protocol screens and Device Settings screen)		Directs the system to accept the current screen entries and to proceed to the next step.
Cancel Session button (various Clinical Protocol screens)		Cancels a treatment session for a particular patient. A prompt is then displayed to confirm your decision.
Return button (various Device Settings screen)		Returns to the Device Settings menu.



CAUTION: Only qualified and experienced personnel shall operate the KXL System.

3.3 UV Dose

- The UV Energy (Dose) is the product of the UV Power (Irradiance) and the UV Irradiation Time. The UV Energy, the UV Power and the UV Irradiation Time are displayed on the user interface.
- The system tracks UV Energy, UV Power, UV Irradiation Time and Total Treatment Time during the treatment.

NOTE - The system's parameters are:

Induction Period:	30 minutes
Wavelength	365 nm
UV Energy:	5.4 J/cm ²
UV Power:	3 ± 10% mW/cm ²
UV Irradiation Time:	30 minutes

3.4 Preparing the System

- Position the KXL System adjacent to the treatment table or chair. Lock the casters to secure the device's position.
- Make sure the system is turned ON.
- Check glass window of beam aperture for dust and dirt. See sections 4.8 and 4.9 for cleaning instructions.

3.5 Important Steps before Turning on the System

- The user is responsible for assuring that the KXL System is functioning properly and is in good working condition before starting a treatment.
- To ensure the system is functioning properly, consider the following mandatory points:
 - Inspect the device, accessories, and connecting cables for visible damage.
 - Take local regulations for use of portable electro-optical medical devices into consideration.

3.6 Powering Up the System

- Turn ON the single power switch on the front of the KXL console. This switch turns on all the system components.



Figure 3-1. Power Switch

The KXL System begins a power-up sequence, loading the operating system and all configuration and reference files.

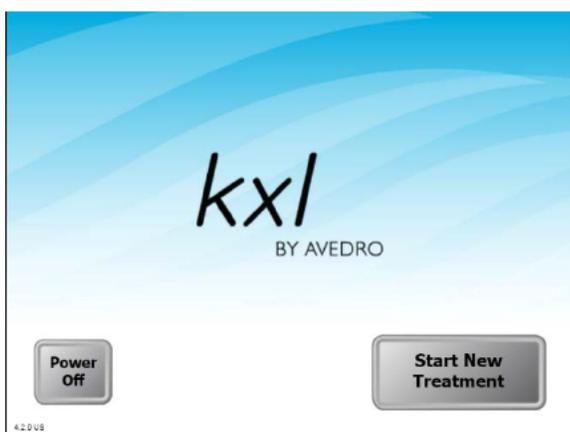


Figure 3-2. Startup Screen

- Please see section 3.20 for Power Down sequence instructions.

NOTE: If there is a Start-up error, please note any error messages and contact your distributor or Customer Service immediately.

3.7 Confirm Riboflavin Induction Period

- To begin patient treatment, press the Start New Treatment button.
- Confirm the length of the induction period (30 min) for the patient.
- To proceed, press the Checkmark button.

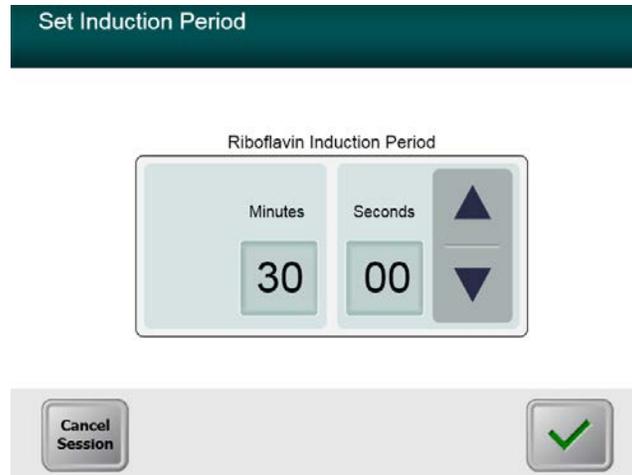


Figure 3-3. Induction Period Screen

3.8 Confirm UV Treatment

3.8.1 Confirm UV Dose

- Confirm the desired UV treatment parameters by pressing the **Checkmark** button:
 - Total Energy (5.4 J/cm²)
 - UV Power (3 mW/cm²)

NOTE: UV irradiation time is displayed in the orange box.



WARNING: The Treatment Activation Card is pre-programmed with above parameters and will only confirm the above energy and power dose.

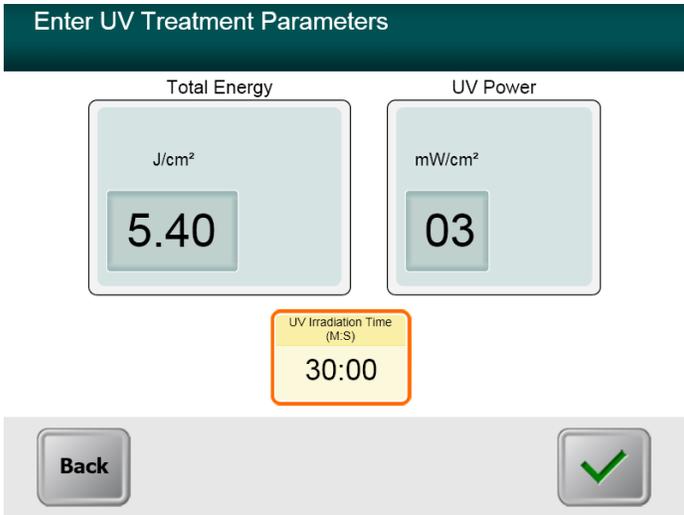


Figure 3-4. UV Energy Dose

- Confirm the specified treatment parameters by pressing the Checkmark.

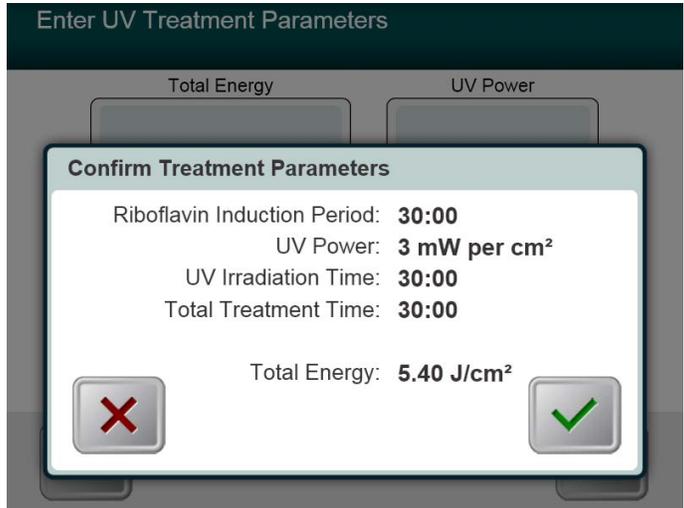


Figure 3-5. Confirm Treatment Parameters Screen

3.9 Starting Treatment

- Place the activation card on the RFID reader and hold in place until the system emits a beep.

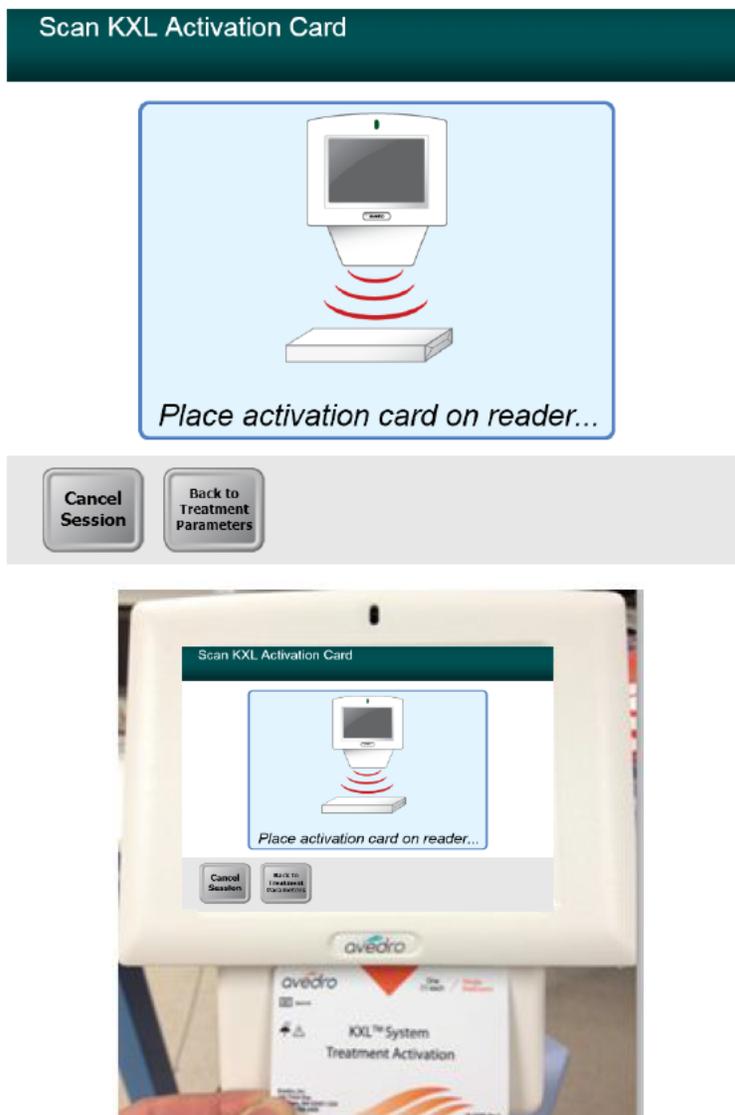


Figure 3-6. Reading Activation Card



WARNING: The Treatment Activation Card is pre-programmed with stated parameters of 3 mW/cm^2 and 5.4 J/cm^2 .

3.9.1 Single-use disposables

- Hold until read is complete and discard tag or activation card.

3.9.2 Multi-use disposables



- Once a multi-use activation card has been scanned, the display will show the number of treatments remaining on the card.

Figure 3-7. Treatments Remaining



Figure 3-8. Final Treatment

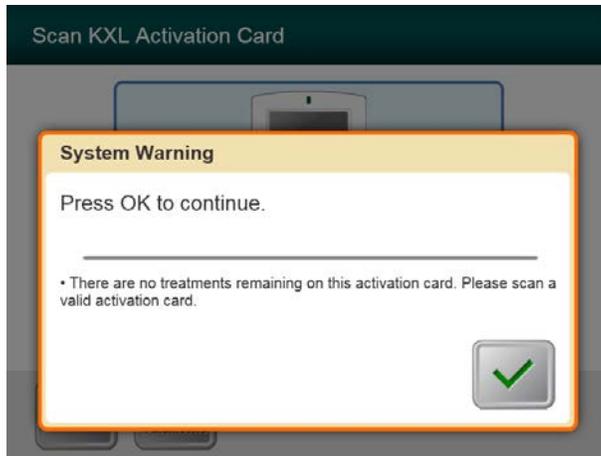


Figure 3-9. No Treatments Remaining

3.9.3 Sync Alignment Remote

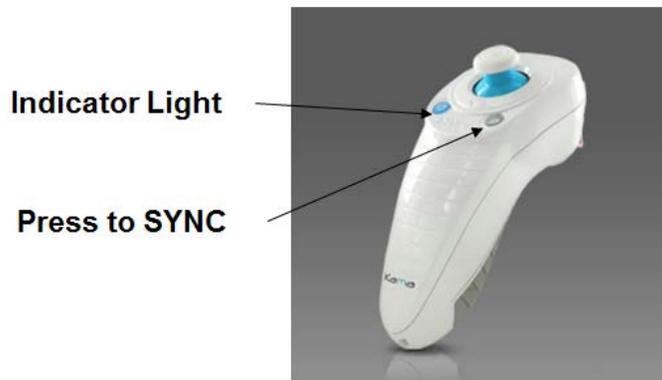
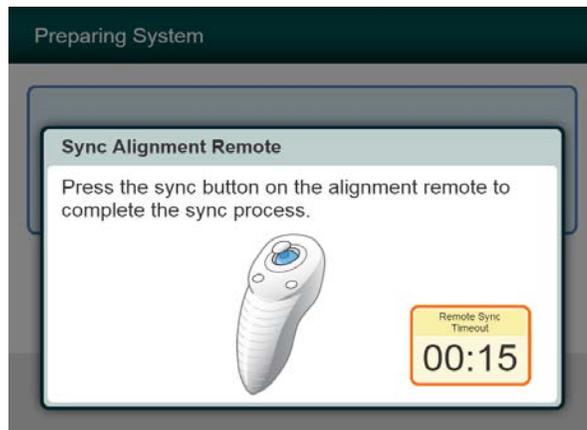


Figure 3-10. Remote Synch Status

- Press the “S” button on the remote to synchronize the remote within the 15 second window displayed on the screen. This is required for every procedure.

Indicator Light Status	Meaning
ON	Actively Synchronized with the device
Blinking once per second for 10 seconds	Disconnecting Sync (After procedure)
Blinking constantly, twice per second	Replace batteries immediately (2 AAA)

NOTE: The KXL system performs an internal self-test prior to each treatment to verify proper UVA calibration. The internal self-test uses a redundant set of optical sensors to ensure that accurate levels of UVA will be delivered for each treatment. If the internal self-test fails, an error message will be generated and the treatment cannot proceed. If this occurs, contact your distributor or Customer Service immediately.

3.10 Preparing the Patient

- Ensure that the patient is lying flat or reclined on a patient table or chair. His or her head should rest in a headrest.
- Adjust the table or chair and headrest so that the patient can rest comfortably for the duration of the treatment without head movement.
- Apply a lid speculum and optional drapes using standard clinical technique.
- Using topical anesthesia, debride the epithelium to a diameter of approximately 9 mm using standard aseptic technique.

3.11 Administration of Photrex Viscous

- Post epithelial debridement, instill 1 drop of PHOTREXA VISCOUS topically on the eye every 2 minutes for 30 minutes.
- **Once the Photrex Viscous is applied to the eye, start the induction by pressing the “Riboflavin Applied: Start Timer” button.**

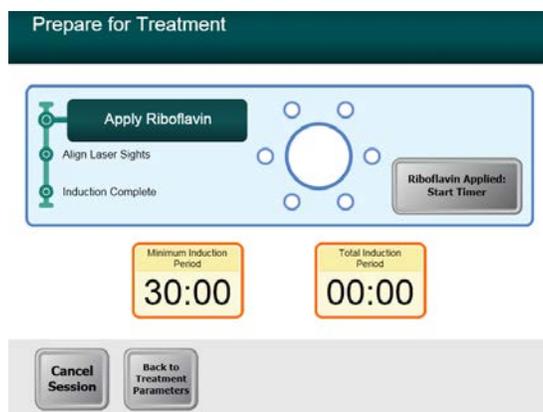


Figure 3-11. Prepare Patient Screen

3.12 Confirm Riboflavin Absorption

When the Induction Time is complete the “Begin UV Treatment” button will appear. Prior to initiating treatment:

- Examine the eye under the slit lamp for the presence of a yellow flare in the anterior chamber.
- If the yellow flare is not detected, instill 1 drop of PHOTREXA VISCOUS every 2 minutes for an additional 2 to 3 drops and recheck for the presence of a yellow flare. This process can be repeated as necessary.

3.13 Confirm Corneal Thickness

- Once the yellow flare is observed, perform ultrasound pachymetry.
- If corneal thickness is less than 400 microns, instill 2 drops of PHOTREXA every 5 to 10 seconds until the corneal thickness increases to at least 400 microns.
- If unable to achieve corneal thickness of at least 400 microns, abort procedure.

3.14 Alignment of the Device

- KXL has two alignment lasers.
 - Red crosshair for X and Y axis positioning.
 - A second red crosshair for Z axis positioning.

Note: For correct alignment when using the Remote, the Avedro logo on optics head should face the user

- Manually move the Optics head back and forth and left and right until the red crosshairs are aligned to the center of the pupil.
- Manually move the Optics head up and down to align the Z axis or second red crosshair to the center of the first red crosshair.
- Fine tune the alignment as needed using the wireless remote.
- The patient should attempt to fixate on the red X & Y alignment crosshair throughout the treatment.

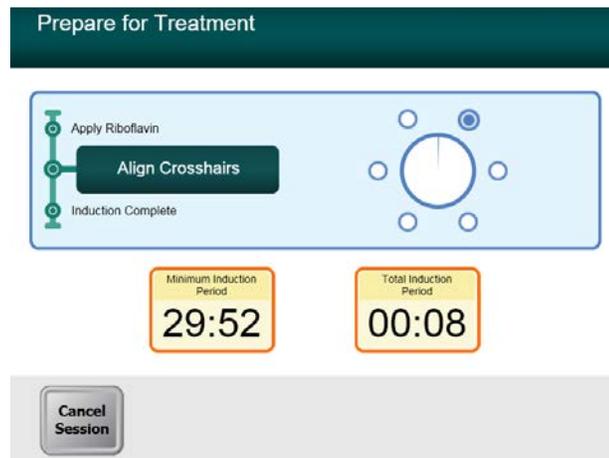


Figure 3-12. Align Crosshairs during induction



Figure 3-13. Remote Functions

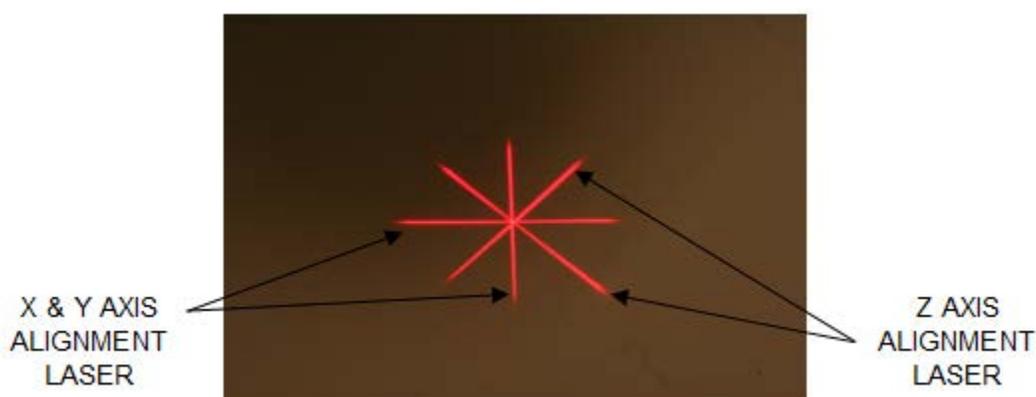


Figure 3-14. Red Crosshairs X & Y Axes, Red Crosshairs Z Axis Alignment

3.15 Initiating Treatment



Irradiation should not be performed unless the 400 micron corneal thickness threshold is met.

- Press the **“Begin UV Treatment”** button to initiate treatment.
- During irradiation, continue topical instillation of PHOTREXA VISCOUS onto the eye every 2 minutes for the 30 minute irradiation period.

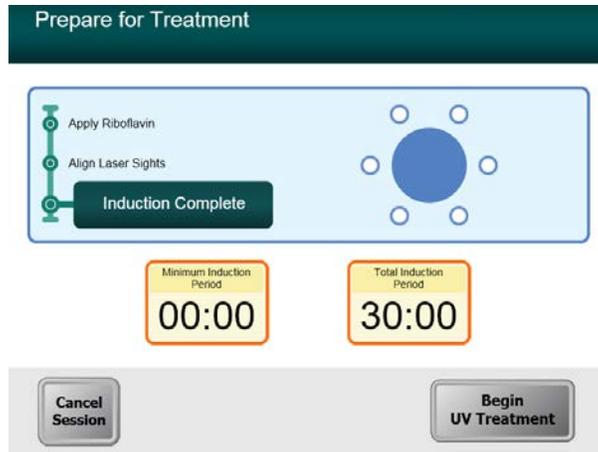


Figure 3-15. Induction Complete

NOTE: The KXL system continuously monitors UVA levels during treatment. The internal monitor uses a redundant set of optical sensors to ensure that accurate levels of UVA are delivered throughout the treatment. If the UVA levels deviate from the intended values, an error message will be generated and the treatment cannot proceed. If this occurs, contact your distributor or Customer Service immediately.



WARNING: Avoid direct illumination of the limbus.



CAUTION: UV light is emitted when the Avedro logo on the optical head changes color from blue to green.



WARNING: Make sure that the KXL System and the patient's table or chair are secured and not moved after alignment and during treatment.

3.16 Monitoring Treatment

- Check continuously that the area of debridement on the cornea is illuminated with the UV light and adjust as necessary using the wireless remote.

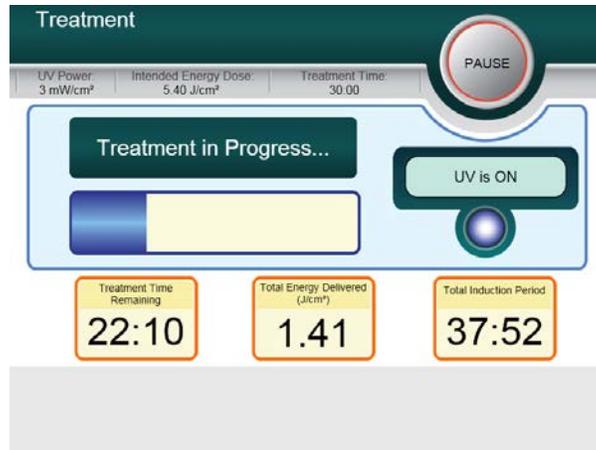


Figure 3-16. Treatment Screen

- The patient should attempt to fixate on the red X & Y alignment crosshair throughout the treatment.
- Patients should remain still during the treatment.

3.17 Stopping a Treatment

- The treatment stops automatically after the treatment timer expires.
- The user may decide to stop or interrupt the treatment. In such case, the UV light can be switched OFF by pushing the **Pause** button.

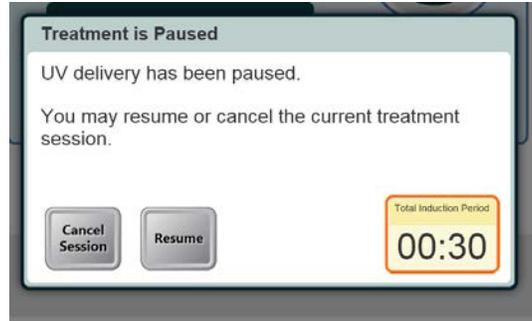


Figure 3-17. Treatment Paused Screen

- To cancel or resume treatment press “Cancel Session” or “Resume” as appropriate. See section 3.19 if canceling a session.

3.18 Treatment Complete

- At the completion of a treatment the Total Treatment Parameters will be displayed and the screen will show Treatment complete. Press **Start New Treatment** to initiate next treatment.



Figure 3-18. Treatment Complete Screen

- To exit treatment and / or start a new treatment press **Start New Treatment**.
- If treatments are complete Power OFF the system using the “Power Off” button on the Main Screen.
- Carefully remove the device from the patient area.
- Remove speculum.

3.19 Pausing or Canceling a Treatment

Treatment may be paused at the discretion of the physician. If a session is **anceled** the following screen displays with **Confirm Cancel Session**.

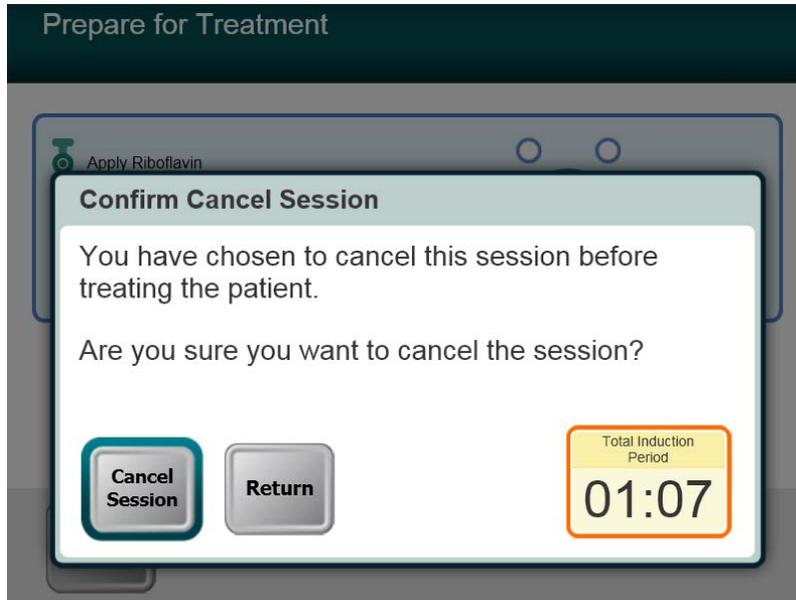


Figure 3-19. Confirm Cancel Session Screen

- To cancel a session press **Cancel Session**.
- If the session is **Paused** the screen displays **Confirm Cancel Partial Treatment**.

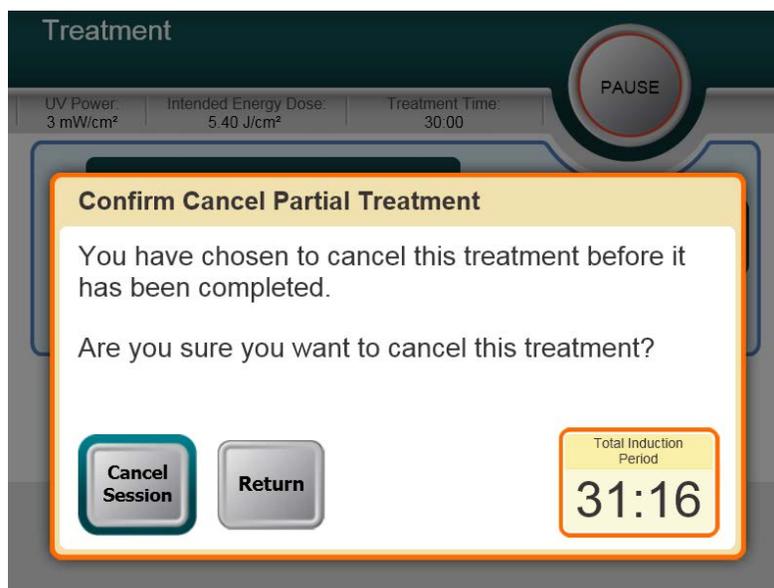


Figure 3-20. Confirm Cancel Partial Treatment

- To cancel the session press **Cancel Session**.

The screen displays **Partial Treatment Information**

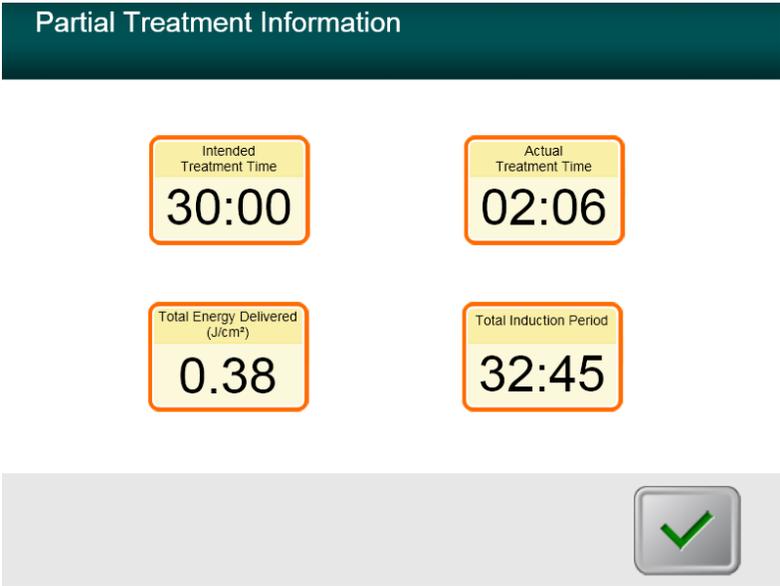


Figure 3-21. Partial Treatment Information

3.20 Powering Down the System

It is recommended that the KXL System be plugged into an electrical outlet when not in use or when stored.



Figure 3-22. Power Off

- Press the “Power Off” on the touch screen monitor.



Figure 3-23. Power Off Position

- Turn the system power switch to the “Off” position.

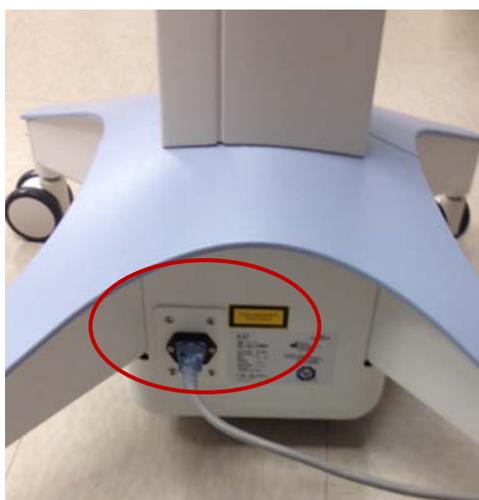


Figure 3-24. KXL System Plug

- Plug the KXL System in to an electrical outlet until next use.

3.21 Using the Device Settings Menu

- With the Initialization screen (Start New Patient) displayed, press and hold the KXL logo on the touch screen.

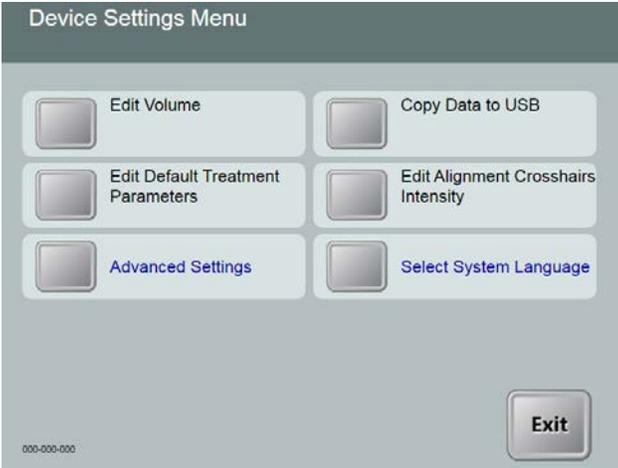


Figure 3-25. Device Settings Menu

3.21.1 Advanced Settings

- Advanced Settings are only available to Avedro and Service personnel with a KXL Advanced Settings access card. If selected the user will be prompted to scan an access card.

3.21.2 Editing System Language

- The System Language option allows a user to select the language of the Graphical User Interface.
- Select the desired language from the dropdown menu.



Figure 3-26. Edit System Language

3.21.3 Editing Alignment Crosshairs Intensity

- The Alignment Crosshairs Intensity option allows a user to edit the brightness of the alignment crosshairs.
- Select the **Edit Alignment Crosshairs Intensity** button on the Device Settings menu.

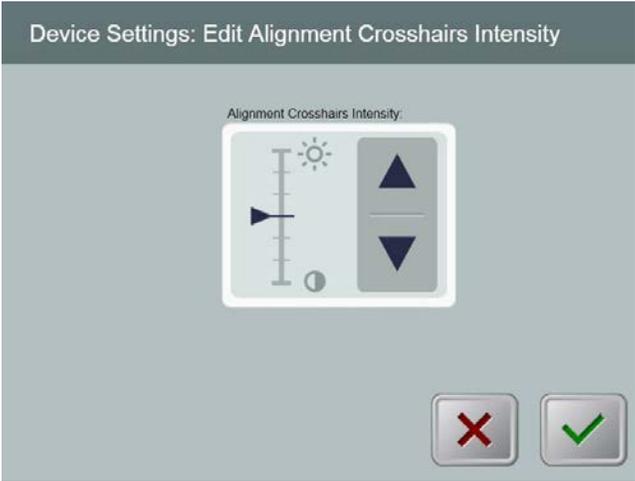


Figure 3-27. Edit Alignment Crosshairs Intensity

3.21.4 Editing System Volume

- The Edit Volume option allows a user with the appropriate security level to edit the system volume level.

- Select the **Edit Volume** button on the Device Settings menu.

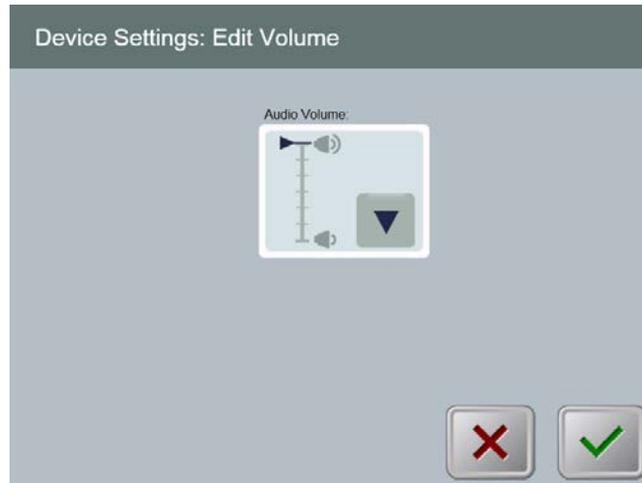


Figure 3-28. Edit Volume

3.21.5 Copying Treatment Data to USB



WARNING: The USB port can only be used when the system is not in treatment mode. Do not have items connected to the USB during treatment.

- Select the **Copy Treatment Data to USB** button on the Device Settings menu.



Figure 3-29. Data Transfer to USB

- Insert a USB device to a USB port and then press the **Copy treatment data to USB** button. The system begins transferring the treatment data and shows a progress bar of the transfer process as shown in the screen below.
- Once complete press the **Return** button. The system will return you to the Device Settings menu.

3.21.6 Confirming Treatment Settings

- The Device Settings: Treatment Parameters option allows a user to confirm the treatment parameters that are displayed on that system.

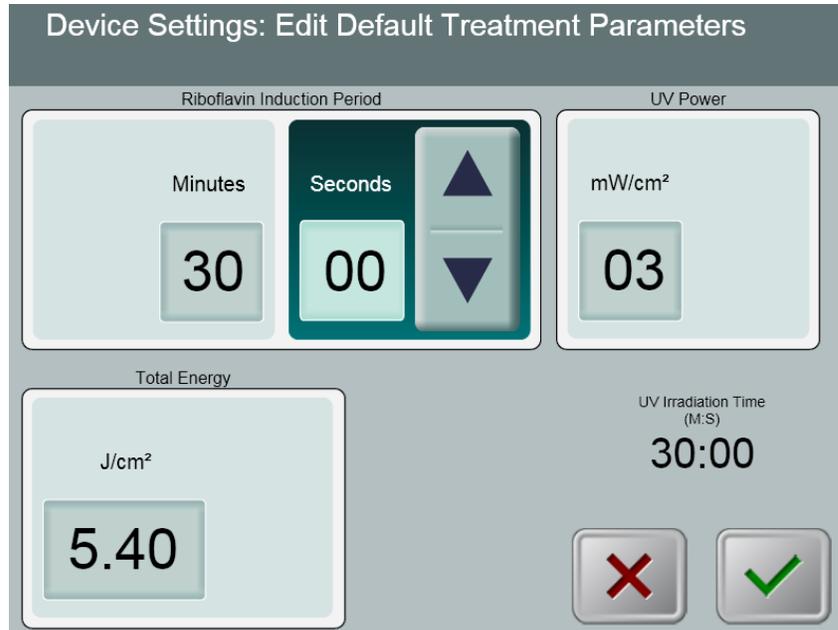


Figure 3-30. Edit Default Treatment Parameters

- When treatment parameters are confirmed, press the **Checkmark** button to exit these Settings.

4 Maintenance / Service

By definition, “maintenance” refers to those non-technical procedures an everyday operator must perform to keep the system working properly. The word “service,” by contrast, refers to tasks that are intended to be performed only by a qualified service representative.

4.1 Installation Policy

- For each new KXL System, a person trained by Avedro can perform a full initial installation and start-up of the system. Following initial installation and once the system is operating properly, the Avedro representative may also provide basic training to a designated operator about the basic operation of the KXL System.
- Consequently, this manual does not include any specific instructions relating to installation or set-up of the system. Per your service agreement, any further hardware adjustment, other than what is specified for normal operation, should be performed by, or with the guidance of, an Avedro-authorized representative.

4.2 Customer Maintenance

- In general, there is no customer maintenance required for The KXL System. All technical maintenance or service will be performed by a qualified service representative while under service contract. If you have trouble with your system, refer to the troubleshooting section below or call your local Avedro Representative.

4.3 Warranty Information

- A Warranty is supplied separately with the purchasing information.

4.4 Service Contract Information

- A service contract is available on all KXL Systems. The contract provides for regularly scheduled maintenance. It also provides for any non-scheduled service calls that may be necessary.

4.5 Troubleshooting

- The KXL System checks its status at start-up automatically. If the status is incorrect, the software prevents the operator from initiating treatments.

Wireless Remote

- The KXL System uses a remote control with replaceable batteries. If the batteries run low the system will lose its connection with the remote and notify the user of the need to re-synchronize and will not allow the user to initiate a procedure. If the remote synchronization is lost during a treatment the user will be prompted to determine if they want to continue the treatment without the remote.

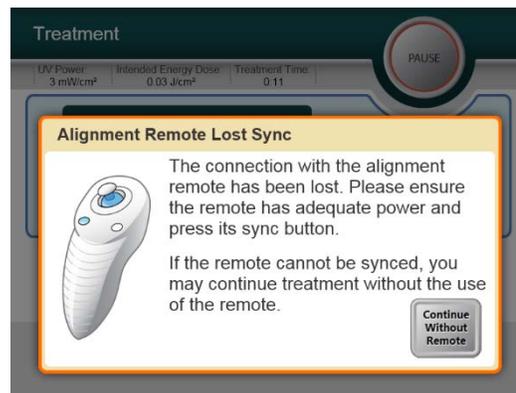


Figure 4-1. Remote Lost Sync

- If light on the remote is flashing two times per second the remote's batteries need to be changed. Replace the batteries prior to initiating a treatment.
- If the light on the remote is flashing once per second then it is not synchronized.
- If the remote does not re-synchronize by pressing the "Sync" button, replace the batteries.
- If replacing the batteries does not allow the system to synchronize contact your local Avedro Service Representative.

Internal Rechargeable Battery

- The KXL system is supplied with a rechargeable battery, if the system does not appear to be turning on ensure that the battery is charged by plugging it into an outlet and checking the charging indicator on the column of the system. If the light is orange or yellow the system is charging, if it is green it is fully charged.
 - If the indicator is green or yellow and the system still does not turn on contact your local Avedro service representative.
 - If the indicator is orange wait until it turns yellow or green and try turning the system on, if it still does not turn on or the indicator does go yellow or green within 8 hours contact your local Avedro service representative.

4.6 Directions for Sterilization or Disinfection

- No components of the KXL System are designed to be sterilized by the operator. External cleaning and disinfection **ONLY** is recommended. For disinfection purposes, use only isopropyl alcohol spray or preparations. Use small amounts of liquid and soft fiber-free wipes.

4.7 Cleaning the System

- Use a soft damp cloth to clean the system.
- The exterior of the KXL System can be cleaned using a lint-free cloth dampened with isopropyl alcohol.
- **DO NOT** submerge the system in liquid or pour liquid onto the system.



CAUTION: Remove the power supply cord from the main outlet and turn off the power switch prior to any cleaning procedure.



CAUTION: The glass window of the beam aperture must not under any circumstances be in contact with any aggressive cleaning agents.

- While cleaning the surfaces of the device, ensure that cleaning fluids do not seep inside the device, as this leakage can damage the device.
- Use a lint-free cloth dampened with isopropyl alcohol to clean the remote control.

4.8 Cleaning the Aperture

- Check the beam aperture routinely prior to treatment.
- Use special camera lens wipes or compressed air to remove dust and particles from the glass surface of the aperture.

4.9 Articulating Arm Adjustment

If the articulating arm does not hold the Optical Head in a fixed vertical position contact your local Avedro service representative.

4.10 Moving the System

- The KXL is designed as a movable system within an office environment. If it ever proves necessary to transport or ship the KXL System, for any reason, contact your local Avedro representative. Packing and transporting the system should be performed only by Avedro trained and authorized personnel.
- Prior to moving the KXL System from one room to another, the monitor should be moved sideways and the optics head should be positioned close to the cart handle with the elbow protruding at the back. The system can then be easily pushed by the cart handle through the door frame.

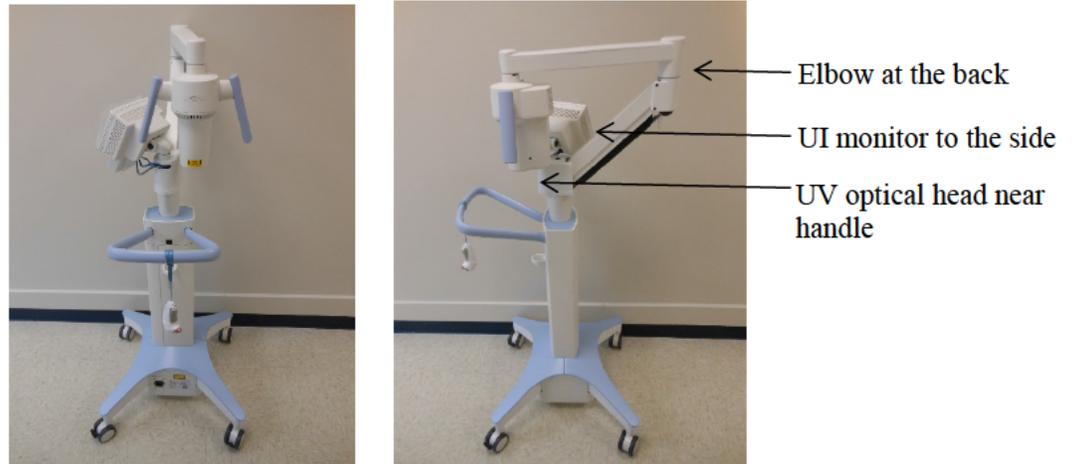


Figure 4-2 Moving System Configuration

4.11 Storing the System

- Follow all the storage temperature and humidity range specifications as listed in the Specifications chapter 7.0.
- Close all panels on the system to prevent dust and moisture from entering; this is mandatory.
- Turn OFF all the components and the main power supply as well. Disconnect the power cord physically from its electrical outlet.
- Remove the batteries from the wireless remote.
- Cover the touch screen LCD display and keyboard with its original cover or packaging to prevent any damage.
- Do not disassemble any part of the system as this could cause misalignment or damage.

4.12 Software

- Should the software become corrupted and fail to work correctly at some point, call your local Avedro service representative. Software updates will only be carried out by Avedro service representatives.

4.13 Identifying Risks Associated with Disposing of Waste Products

- When disposing of waste products, follow all applicable local regulations.

4.14 Performing a Visible Check

- Check all components of the device routinely for damage or malfunction prior to each treatment.
- Do not use a damaged or malfunctioning device. Use of such devices may harm the user and/or patient.

5 Equipment Classification

5.1 Essential Performance

The KXL system delivers to the cornea UV-A radiation of nominally 365 nm wavelength at an irradiance of 3 mW/cm² over an exposure period of up to 30 minutes to deliver a total energy density of up to 5.4 J/cm².

5.2 Equipment Classification

According to IEC60601-1 Medical Device Electrical Standard

- Protection against electrical shock
 - Class 1 (external electrical power source)
 - Internally powered equipment (internal battery operation)
- Degree of protection against electric shock
 - Not classified, equipment not provided with applied part
 - Ingress protection: IP20
- Method of sterilization or disinfection
 - Disinfect-able device
- Degree of protection for use in the presence of a flammable anesthetic mixture
 - No protection
- Use conditions
 - Continuous service

According to FCC Part 15, IEC55011 and IEC60601-1-2

- Class B

According to IEC60825-1 Safety of laser productions

- Alignment lasers are Class 1 Laser Product

According to IEC62471 Photobiological safety of lamps and lamp systems

- UVA LED is Risk Group 1

According to Annex II.3 of Directive 93/42/EEC

- Class IIa

5.3 EMC Guidance

Guidance and manufacturer's declaration - electromagnetic emissions		
The KXL UV Illumination System is intended for use in the electromagnetic environment specified below. The customer or the user of the KXL UV Illumination System should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment — guidance
RF emissions CISPR 11	Group 1	The KXL UV Illumination System uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The KXL UV Illumination System is suitable for use in all establishments other than domestic, and may be used in domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes, provided the following warning is heeded: Warning: This equipment/system is intended for use by healthcare professionals only. This equipment/system may cause radio interference or may disrupt the operation of nearby equipment. It may be necessary to take mitigation measures, such as re-orienting or relocating the KXL UV Illumination System or shielding the location.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/ flicker emissions IEC 61000-3-3	Complies	

Table 5-1

Guidance and manufacturer's declaration — electromagnetic immunity			
The KXL UV Illumination System is intended for use in the electromagnetic environment specified below. The customer or the user of the KXL UV Illumination System should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines Not Applicable Input /Output Lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV line(s) to line(s) ±2 kV line(s) to earth	±1 kV line(s) to line(s) ±2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5% U_T (>95% dip in U_T) for 0.5 cycle 40% U_T (60% dip in U_T) for 5 cycles 70% U_T (30% dip in U_T) for 25 cycles <5% U_T (>95% dip in U_T) for 5 sec	0% U_T for 0.5 cycles 40% U_T for 5 cycles 70% U_T for 25/30 cycles 0% U_T for 250/300 cycles	Mains power quality should be that of a typical commercial or hospital environment, If the user of the KXL UV Illumination System requires continued operation during power mains interruptions, it is recommended that the KXL UV Illumination System be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE U_T is the a.c. mains voltage prior to application of the test level.			

Table 5-2

Guidance and manufacturer's declaration – electromagnetic immunity			
The KXL UV Illumination System is intended for use in the electromagnetic environment specified below. The customer or the user of the KXL UV Illumination System should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment — guidance
Conducted RF IEC61000-4-6	3 Vrms 150 kHz to 80 MHz	3 Vrms	Portable and mobile RF communications equipment should be used no closer to any part of the KXL UV Illumination System, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d = 1.2\sqrt{P}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.5 GHz	3 V/m	$d = 1.2\sqrt{P}$ 80 MHz to 800 MHz $d = 2.3\sqrt{P}$ 80 MHz to 2.5 GHz
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment — guidance
			where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, ^a should be less than the compliance level in each frequency range. ^b Interference may occur in the vicinity of equipment marked with the following symbol: 
NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.			
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			
a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the KXL UV Illumination System is used exceeds the applicable RF compliance level above, the KXL UV Illumination System should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the KXL UV Illumination System.			
b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.			

Table 5-3

Recommended separation distances between portable and mobile RF communications equipment and the KXL UV Illumination System			
The KXL UV Illumination System is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the KXL UV Illumination System can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the KXL UV Illumination System as recommended below, according to the maximum output power of the communications equipment.			
Rated maximum output power of transmitter (W)	Separation distance according to frequency of transmitter (m)		
	150 kHz to 80 MHz $d = 1.2\sqrt{P}$	80 MHz to 800 MHz $d = 1.2\sqrt{P}$	800 MHz to 2.5 GHz $d = 2.3\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23
For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.			
NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.			
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			

Table 5-4

5.4 RF Transmitters

5.4.1 RFID reader:

- 13.56MHz Reader/Writer
- Integral Antenna: Maximum 4” Read Range
- US/FCC number SX90RFID1
- Max output power is 200mW
- Meets: ISO18000-3, ISO15693

The highest emissions generated by the above equipment are listed below:

Fundamental	Frequency (MHz)	Level (dB μ V/m) at 30 m	Limit (dB μ V/m) at 30 m	Limit (μ V/m) at 30 m	Margin (dB)
Paragraph 15.225(a)	13.56 (peak)	29.8	84	15,848	-54.2


Other	Frequency (MHz)	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)
Harmonics	27.12 (peak)	-5.2	29.5	-34.7
Spurious	200.6 (peak)	34.5	40.0	-5.5
Conducted	0.199 (avg)	38.8	54.6	-15.8




Table 5-5

5.4.2 Wireless remote control:

- FCC ID SXJ87027-T
- Frequency Range 2402MHz to 2476MHz
- Max Effective power: 0.501mW

6 Symbol Library

Text Symbol	Symbol Illustration	Definition
1. No AP symbol in presence of flammable anesthetics		Danger, Risk of Explosion. Not for use
2. AC symbol		Alternating current
3. "I" in a book		Attention: Consult ACCOMPANYING DOCUMENTS
4. Ground symbol in circle		Protected earth (ground)
5. Power Switch		ON
6. Power Switch		OFF
7. Fuse symbol		Fuse
8. Manufacturer		Name and address of the manufacturer
9. ! in a Triangle		Caution specific warning in operators manual
10. Net Weight (kgs) Gross Weight (kgs)	NW GW	Weight
11. Umbrella with raindrops		Keep Dry: Store protected from moisture (symbol is with or without rain drops)
12. Wine glass with crack on it		Contents are fragile, handle with care

Text Symbol	Symbol Illustration	Definition
13. Two up arrows		Keep arrows on carton pointing up
14. Water drop in a box		Humidity limits (percentages below symbol are the acceptable range for humidity)
15. Temperature limits		Temperature shipment limits
16. MR crossed in a circle		MR Unsafe – Keep away from magnetic resonance imaging (MRI) equipment
17. Signal emitted		This device includes RF transmitters
18. Pressure limits		Atmospheric pressure limits (storage / operating)

7 Specifications

Specification	Description
Electrical	Battery Powered: 12V 35 Ah SLA Line voltages 100 – 240 volts AC Current: 2A – 1A Single Phase RMS, 50/60 Hz Remote 2x AAA batteries
User accessible Fuses	250 V~ T2AH
Energy Delivery	UV Radiation 3 mW/cm ² ±10% 365 nm
UVA LED Light Source	UV Radiation 365 nm
External Interfaces	USB 2.0
Physical Dimensions	No larger than 60 x 60 x 150 cm ³ (Length x Width x Height)
Weight (crated system)	NW 45 Kg GW 120 Kg
System Battery Life (normal operating conditions)	16 hours
Remote Battery Life (normal operating conditions)	18 hours
Environmental Operating Conditions	The system operates under the following atmospheric conditions (no condensation).
Ambient temperature	+10 to +40 °C
Relative humidity	30% to 75%, non-condensing
Atmospheric pressure	700 to 1060 mbar
Transport and Storage Conditions	The instrument withstands the following transport and storage conditions without damage or performance deterioration.
Ambient temperature	-15 to +70 °C
Relative humidity	10% to 100% non-condensing
Atmospheric pressure	500 to 1060 mbar

This is a representation of an electronic record that was signed electronically and this page is the manifestation of the electronic signature.

/s/

WILEY A CHAMBERS
04/15/2016

RENATA ALBRECHT
04/15/2016